



**San Joaquin Valley Air Pollution Control District**

**DRAFT 2018 Air Monitoring Network Plan**

**May 29, 2018**

This page is intentionally blank.

**TABLE OF CONTENTS**

The District’s Core Values Exhibited in the Air Monitoring Network .....	vi
<b>EXECUTIVE SUMMARY</b> .....	1
<b>AIR MONITORING NETWORK PLAN REQUIREMENTS</b> .....	3
Monitoring Objectives, Site Types, and Spatial Scales .....	7
Meteorology .....	8
State of the Air Monitoring Network.....	8
<b>POLLUTANT MONITORING REQUIREMENTS</b> .....	11
Ozone .....	11
Photochemical Assessment Monitoring Stations .....	12
Nitrogen Dioxide.....	13
Carbon Monoxide.....	14
Sulfur Dioxide.....	15
Reactive Nitrogen Compounds (NO <sub>y</sub> ).....	16
Toxics.....	16
Detailed Site Information – Gaseous Monitors.....	17
Particulate Matter (PM) .....	19
Detailed Site Information – PM Monitors.....	20
PM Collocation Requirements.....	21
Public Review of Changes to the PM <sub>2.5</sub> Monitoring Network .....	21
PM <sub>10</sub> Monitoring Requirements.....	21
PM <sub>2.5</sub> Monitoring Requirements.....	23
PM <sub>2.5</sub> Chemical Speciation Site Requirements.....	25
Lead .....	29
NCore.....	29
Non-EPA Federal Monitors .....	30
<b>IMPROVEMENTS AND PLANNED CHANGES TO THE DISTRICT’S AIR MONITORING NETWORK</b> .....	36
Network Changes during 2017/2018.....	36
Planned Improvements and Other Changes Scheduled for 2018/2019 .....	36
<b>DATA SUBMISSION REQUIREMENTS</b> .....	41
<b>ACRONYMS AND ABBREVIATIONS</b> .....	42

## **APPENDICES**

Appendix A: Monitoring Site Descriptions

Appendix B: Detailed SJV Monitoring Site Information

Appendix C: San Joaquin Valley Air Pollution Control District Notice of Public  
Inspection Period on the 2018 Air Monitoring Network Plan

## LIST OF FIGURES

Figure 1	Map of Air Monitoring Sites in the San Joaquin Valley .....	2
----------	---	---

## LIST OF TABLES

Table 1	Types of Air Monitoring Stations, Monitors, and Networks .....	3
Table 2	San Joaquin Valley Areas of Representation .....	5
Table 3	Site Identification .....	5
Table 4	San Joaquin Valley 2017 Population .....	7
Table 5	Parameters Monitored in the San Joaquin Valley .....	9
Table 6	San Joaquin Valley Stations Monitoring Meteorology .....	10
Table 7	SLAMS Minimum Ozone Monitoring Requirements .....	11
Table 8	Ozone Monitoring Requirements for the Valley .....	12
Table 9	San Joaquin Valley PAMS Network .....	13
Table 10	Valley SO <sub>2</sub> PWEI Values for 2017 .....	15
Table 11	Gaseous Monitors .....	17
Table 12	Gaseous Monitors – Monitor Type .....	18
Table 13	Minimum PM <sub>10</sub> Monitoring Requirements* .....	22
Table 14	PM <sub>10</sub> Monitoring Requirements for the Valley .....	22
Table 15	24-Hour PM <sub>10</sub> highest concentrations at each site* .....	23
Table 16	Minimum PM <sub>2.5</sub> Monitoring Requirements.....	23
Table 17	PM <sub>2.5</sub> Monitoring Requirements for the Valley* .....	24
Table 18	24-Hour and Annual PM <sub>2.5</sub> Maximum Design Values .....	25
Table 19	PM <sub>2.5</sub> Speciation Monitors.....	26
Table 20	PM Monitors .....	27
Table 21	PM Monitors – Monitor Type .....	28
Table 22	Fresno-Garland NCore Site.....	30
Table 23	Non–EPA Federal Monitors.....	31
Table 24	SLAMS – Site Type .....	31
Table 25	SLAMS – Spatial Scale .....	32
Table 26	SLAMS – Basic Monitoring Objective .....	33
Table 27	SPM (PM <sub>2.5</sub> Continuous).....	35
Table 28	Summary of Proposed Changes to the Air Monitoring Network .....	39

## **The District's Core Values Exhibited in the Air Monitoring Network**

### **\* Protection of Public Health \***

The District uses data collected from the air monitoring network to provide real-time air quality data to the public through the Real-Time Air Advisory Network (RAAN), generate daily air quality forecasts, and when needed, issue health advisories. The District also uses data collected from the Valley's air monitoring network as the basis for long-term attainment strategies and to track progress towards meeting federal health-based air quality standards.

### **\* Active and effective air pollution control efforts with minimal disruption to the Valley's economic prosperity \***

The District uses air monitoring data to help establish strategies for reaching attainment of federal health-based air quality standards.

### **\* Outstanding Customer Service \***

#### **\* Accountability to the public \***

The District's website provides easy public access to data from the Valley's real-time air monitors, and through the RAAN system, provides notifications to the public when air quality reaches unhealthy levels. The public can also access historical air quality information through the District's website.

### **\* Open and transparent public processes \***

In addition to making air quality data available in real-time, the District uses air quality data in a variety of publicly available documents and reports. The District also conducts a public review period for annual monitoring network plans.

### **\* Respect for the opinions and interest of all Valley residents \***

The District has actively made daily air quality information available to Valley residents in a variety of formats, including the District website, the RAAN system, the daily air quality forecast, and the media. The District considers public interests in establishing new air monitoring stations.

### **\* Ingenuity and innovation \***

The District strives to use new and improved air monitoring techniques and equipment as approved by the EPA. The District uses the latest science when considering locations for air monitoring stations, and in turn, the data collected from the air monitoring network contributes to ongoing scientific evaluations.

### **\* Continuous improvement \***

Through the annual air monitoring network plan, the District evaluates the air monitoring network for opportunities for better data collection and greater efficiency. Throughout the year, the District continually seeks out opportunities to improve the air monitoring network and its service to the public while meeting federal requirements.

### **\* Recognition of the uniqueness of the San Joaquin Valley \***

The San Joaquin Valley is an expansive and diverse area. The District strives to site its air monitoring stations in locations that represent each region of the Valley.

### **\* Effective and efficient use of public funds \***

The District makes the most of limited resources by structuring the air monitoring network in a way that optimizes personnel time and funding for instruments. The result is a robust air monitoring network that helps the Valley reach its air quality goals without unnecessary expenditures.

This page is intentionally blank.



## EXECUTIVE SUMMARY

The San Joaquin Valley Air Pollution Control District (SJVAPCD or District) operates an extensive network of air quality monitors throughout the San Joaquin Valley (Valley) to support its mission of improving and protecting public health. District staff use hourly readings from real-time monitors to communicate the state of the air quality to Valley residents. Through programs and venues such as the Real-Time Air Advisory Network (RAAN), the daily air quality forecast, the District and California Air Resources Board (ARB) websites, and Valley media, residents are able to obtain air quality information that can help them with their activity planning. The District also uses real-time air quality data to manage prescribed burning, hazard reduction burning, agricultural burning, and residential wood burning to ensure these activities do not result in adverse air quality impacts.


As part of the District's long-term efforts to improve public health, air monitors collect data that is rigorously analyzed by laboratory technicians and District staff. This monitoring data determines the Valley's air quality and is fundamental in the Valley's effort to improve air quality and achieve attainment of the Environmental Protection Agency's (EPA's) health-based ambient air quality standards as quickly as possible.

The Valley covers an area of 23,490 square miles, and is prone to one of the most challenging air quality problems in the nation. The Valley is home to 4,000,000 residents and includes several major metropolitan areas, vast expanses of agricultural land, industrial sources, highways, and schools. The Valley is designated as an attainment area for the federal Lead (Pb), Nitrogen Dioxide (NO<sub>2</sub>), Sulfur Dioxide (SO<sub>2</sub>), and Carbon Monoxide (CO) National Ambient Air Quality Standards (NAAQS or standards). In addition, the Valley is designated as an attainment/maintenance area for the PM<sub>10</sub> NAAQS (particulate matter less than 10 microns in diameter). The Valley is designated as a nonattainment area for federal PM<sub>2.5</sub> and ozone (O<sub>3</sub>) standards. To address the air quality needs of this expansive and diverse region, the District maintains a robust air monitoring program that meets federal requirements while providing vital information to the public.

The air monitoring network in the Valley also includes air monitoring stations that are managed and operated by ARB and the National Park Service. Additionally, there are three tribal air monitoring stations operating in the Valley: the Tachi Yokut Tribe operates the Santa Rosa Rancheria air monitoring station located in Kings County; the Monache Tribe and Foothill Yokut Indians operate the air monitoring station located at Table Mountain Rancheria in Fresno County; and the Chukchansi Indians of California operate the Picayune Rancheria air monitoring station located in Madera County. Since the tribal monitors are operated under the Tribal Authority Rule which is essential to tribal implementation of the Clean Air Act (CAA), and are not part of the District's jurisdiction, detailed site information for tribal monitors is not provided in this air monitoring network plan.

A map of the air monitoring sites in the Valley is provided in Figure 1 on the following page.

Figure 1: Map of Air Monitoring Sites in the San Joaquin Valley

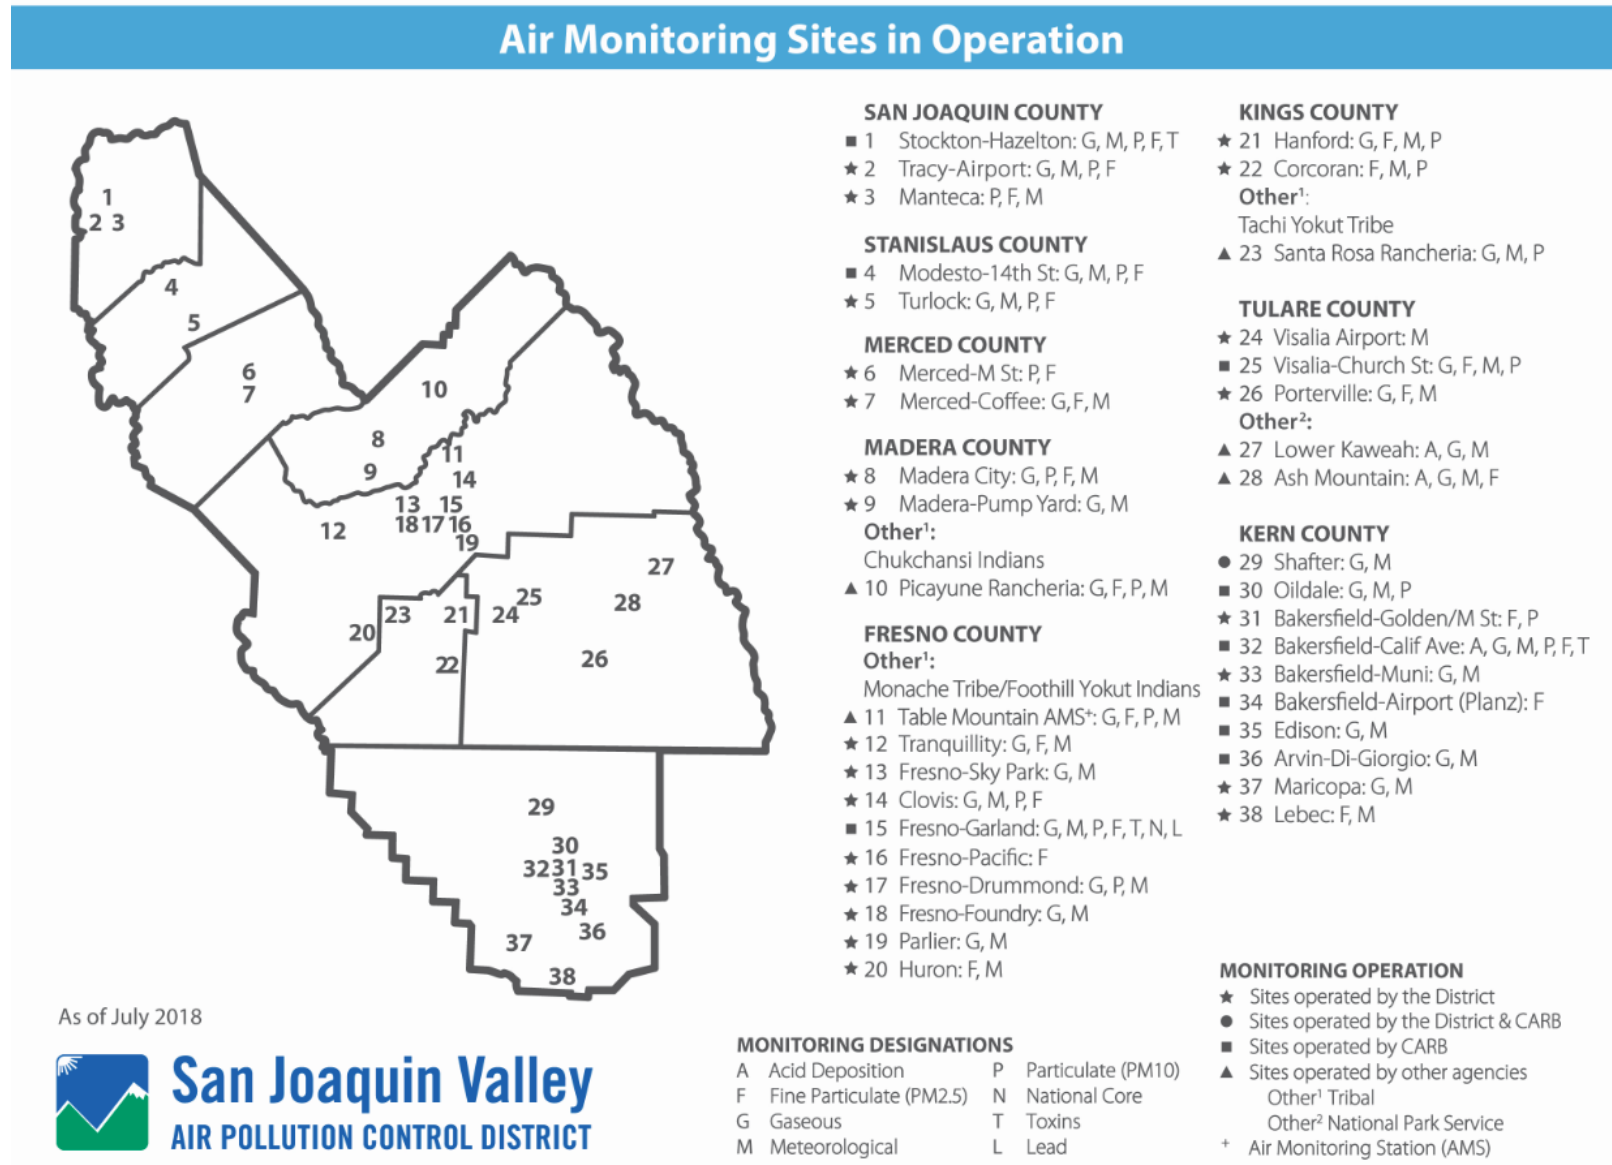

## AIR MONITORING NETWORK PLAN REQUIREMENTS

As specified in Title 40 Code of Federal Regulations (CFR) Part 58, Section 58.10 (40 CFR §58.10), and as a requirement of the District's EPA 105 Grant, this air monitoring network plan describes the current state of the District's monitoring network and planned changes to the network.

Each year, the District updates the air monitoring network plan and posts it for public inspection for at least 30 days prior to submitting it to the EPA Regional Administrator. Air monitoring network plans provide information on the establishment and maintenance of air monitoring networks that may include the types of stations and monitors listed in Table 1.

**Table 1 Types of Air Monitoring Stations, Monitors, and Networks**

Abbreviation	Full Name	Description
FEM	Federal Equivalent Method	These monitors are considered to be equivalent to FRM monitors for the purpose of determining compliance with EPA's health-based air quality standards.
FRM	Federal Reference Method	EPA defines how these monitors are to work, how they are to be engineered, and how they are to measure pollutants. These monitors are used to determine compliance with EPA's health-based air quality standards.
NCORE	National Core	Multipollutant monitoring stations; in California, these are operated by CARB.
PAMS	Photochemical Assessment Monitoring Station	VOC (volatile organic compounds) speciation sites used in serious, severe, or extreme ozone nonattainment areas for precursor evaluation.
SLAMS	State and Local Air Monitoring Station	Monitoring sites that are used for determinations of compliance with federal air quality standards, though they may be used for other purposes as well.
SPM	Special Purpose Monitor	Not included when showing compliance with the minimum air monitoring requirements; an example might include a temporary monitoring station set up in an area to measure short term air quality impacts of a source. Data collected from an SPM can be used for Regulatory purposes if the monitor has been operational for two years and if the monitor is an ARM, FEM, or FRM.
STN	Speciated Trends Network	PM <sub>2.5</sub> speciation stations that provide chemical speciation data of PM.

The air monitoring network plan should include a statement of purpose for each monitor and evidence that siting and operation of each monitor meets the requirements of Appendices A, C, D, and E of 40 CFR Part 58. The plan must contain the following information for each existing and proposed site (40 CFR §58.10 (b)):

- The MSA, CBSA, CSA, or other area represented by the monitor. MSA, CBSA, and CSA are statistical-based definitions for metropolitan areas provided by the Office of Management and Budget and the Census Bureau (see Table 2):
  - MSA: Metropolitan statistical area
  - CBSA: Core-based statistical area
  - CSA: Combined statistical area
- Air Quality System (AQS) site identification number (see Table 3).
- Population estimate (see Table 4).
- Location: Street address and geographical coordinates (see Appendix B).
- Sampling and analysis methods for each measured parameter (see Appendix B).
- Operating schedules for each monitor (see Appendix B).
- Monitoring objective and spatial scale of representativeness for each monitor (as defined in Appendix D to 40 CFR Part 58) (see Appendix B).
- Any proposals to remove or move a monitoring station within 18 months of a plan submittal. Any proposed additions and discontinuations of SLAMS monitors are subject to approval according to 40 CFR §58.14 (see *Improvements and Planned Changes* section of this document).

There are several network plan requirements that pertain specifically to PM<sub>2.5</sub> monitoring:

- The monitoring network plan must identify which sites are suitable and which are not suitable for comparison against the annual PM<sub>2.5</sub> NAAQS as described in 40 CFR §58.30 (see *PM<sub>2.5</sub> Monitors* section of this document).
- The plan must also document how the District provides for public review of changes to the PM<sub>2.5</sub> monitoring network when the change impacts the location of a violating PM<sub>2.5</sub> monitor, or the creation/change to a community monitoring zone.
- The District should submit any public comments received on PM<sub>2.5</sub> monitoring changes in the submittal of the air monitoring network plan.
- On March 18, 2013, EPA finalized the rule to revoke the term “population-oriented.” The final rule states that PM<sub>2.5</sub> monitors at neighborhood scale or larger, or smaller scales that represent many locations in the same CBSA, are the only monitors representative of “area-wide” air quality that can be compared to the PM<sub>2.5</sub> NAAQS.

**Table 2 San Joaquin Valley Areas of Representation**

TITLE	CODE
<b>Combined Statistical Area (CSA)</b>	<b>Combined Statistical Area (CSA) Code</b>
Fresno–Madera	260
<b>Metropolitan Statistical Area (MSA)</b>	<b>Core–Based Statistical Area (CBSA) Code</b>
Stockton–Lodi	44700
Modesto	33700
Merced	32900
Madera	31460
Fresno	23420
Hanford–Corcoran	25260
Visalia–Porterville	47300
Bakersfield*	12540

Monitors from both the District and the Eastern Kern County Air Pollution Control District can be counted when determining compliance with minimum monitoring requirements for the Bakersfield CBSA. However, only monitors located within the District's boundaries are included in this network plan.

**Table 3 Site Identification**

<b>MSA/CBSA: Stockton-Lodi</b>		
<b>County: San Joaquin</b>		
<b>Site Name</b>	<b>AQS ID</b>	<b>Operating Agency</b>
Manteca	06-077-2010	SJVAPCD
Stockton–Hazelton	06-077-1002	CARB
Tracy–Airport	06-077-3005	SJVAPCD
<b>MSA/CBSA: Modesto</b>		
<b>County: Stanislaus</b>		
<b>Site Name</b>	<b>AQS ID</b>	<b>Operating Agency</b>
Modesto–14th St	06-099-0005	CARB
Turlock	06-099-0006	SJVAPCD
<b>MSA/CBSA: Merced</b>		
<b>County: Merced</b>		
<b>Site Name</b>	<b>AQS ID</b>	<b>Operating Agency</b>
Merced–Coffee	06-047-0003	SJVAPCD
Merced–M St	06-047-2510	SJVAPCD
<b>MSA/CBSA: Madera</b>		
<b>County: Madera</b>		
<b>Site Name</b>	<b>AQS ID</b>	<b>Operating Agency</b>
Madera–City	06-039-2010	SJVAPCD
Madera–Pump Yard	06-039-0004	SJVAPCD

**Table 3 Site Identification (continued)**

<b>MSA/CBSA: Fresno</b>		
<b>County: Fresno</b>		
<b>Site Name</b>	<b>AQS ID</b>	<b>Operating Agency</b>
Clovis–Villa	06-019-5001	SJVAPCD
Fresno–Drummond	06-019-0007	SJVAPCD
Fresno–Garland	06-019-0011	CARB
Fresno–Foundry	06-019-2016	SJVAPCD
Fresno–Pacific	06-019-5025	SJVAPCD
Fresno–Sky Park	06-019-0242	SJVAPCD
Huron	06-019-2008	SJVAPCD
Parlier	06-019-4001	SJVAPCD
Tranquillity	06-019-2009	SJVAPCD
<b>MSA/CBSA: Hanford–Corcoran</b>		
<b>County: Kings</b>		
<b>Site Name</b>	<b>AQS ID</b>	<b>Operating Agency</b>
Corcoran–Patterson	06-031-0004	SJVAPCD
Hanford–Irwin	06-031-1004	SJVAPCD
<b>MSA/CBSA: Visalia–Porterville</b>		
<b>County: Tulare</b>		
<b>Site Name</b>	<b>AQS ID</b>	<b>Operating Agency</b>
Porterville	06-107-2010	SJVAPCD
Sequoia–Ash Mountain	06-107-0009	National Park Service
Sequoia–Lower Kaweah	06-107-0006	National Park Service
Visalia–Airport	06-107-3000	SJVAPCD
Visalia–Church St	06-107-2002	CARB
<b>MSA/CBSA: Bakersfield</b>		
<b>County: Kern (Valley Portion)</b>		
<b>Site Name</b>	<b>AQS ID</b>	<b>Operating Agency</b>
Arvin–Di Giorgio	06-029-5002	CARB
Bakersfield–Golden / M St	06-029-0010	SJVAPCD
Bakersfield–California	06-029-0014	CARB
Bakersfield–Muni	06-029-2012	SJVAPCD
Bakersfield–Airport (Planz)	06-029-0016	CARB
Edison	06-029-0007	CARB
Lebec	06-029-2009	SJVAPCD
Maricopa	06-029-0008	SJVAPCD
Oildale	06-029-0232	CARB
Shafter	06-029-6001	Shared *

\*Site operated by CARB and SJVAPCD.

**Table 4 San Joaquin Valley 2017 Population**

County	Total County Population*	Major Urban Area Pop > 100,000	Urban Area Pop < 100,000 and > 50,000
San Joaquin	746,868	Stockton	Lodi, Manteca, Tracy
Stanislaus	548,057	Modesto	Turlock
Merced	274,665	—	Merced
Madera	156,492	—	Madera
Fresno	995,975	Fresno, Clovis	—
Kings	149,537	—	Hanford
Tulare	471,842	Visalia	Porterville, Tulare
Kern (Valley Portion)	760,845**	Bakersfield	Delano
Kern (Entire County)	895,112	Bakersfield	Delano
<b>San Joaquin Valley Total</b>	<b>4,104,281</b>		

\* Data from California Department of Finance E-1 Population Estimates for Cities, Counties and the State, January 1, 2017, Released May 1, 2017

\*\* Population estimate for Kern County (Valley Portion) was calculated using census tract data for the population living within the District's boundaries. The San Joaquin Valley Total includes the Kern (Valley Portion) population and not the Kern (Entire County) population.

### Monitoring Objectives, Site Types, and Spatial Scales

Three **basic monitoring objectives** that define the purpose of each analyzer are identified in 40 CFR Part 58 Appendix D:

- Provide air pollution data to the general public in a timely manner (**timely/public**).
- Support compliance with ambient air quality standards and emissions strategy development (**NAAQS comparison**).
- Support for air pollution research studies (**research support**).

**Site types** meet the objectives that define what the monitor is measuring. Some of the general monitoring site types identified in 40 CFR Part 58, Appendix D include:

- Sites located to determine the **highest concentrations** in the area covered by the network.
- **Population exposure** sites to measure typical concentrations in areas of high population density.
- **Source oriented** sites to determine the impact of significant sources or source categories on air quality.
- **General Background** sites determine background concentration levels.
- **Regional transport** sites located to determine the extent of regional pollutant transport among populated areas and in support of secondary standards
- Sites located to measure air pollution impacts on visibility, vegetation damage, or other welfare-related impacts.

Scales of spatial representativeness are described in terms of physical dimensions of the air parcel or zone where air quality is expected to be reasonably consistent around the monitor. The monitor thus represents that area, not just the point of the monitor. The following **spatial scales** are identified in 40 CFR Part 58, Appendix D:

- **Microscale:** An area ranging from several meters up to about 100 meters.
- **Middle scale:** An area covering between about 100 meters to 0.5 kilometers.
- **Neighborhood scale:** Covering an area between 0.5 and 4.0 kilometers in range.
- **Urban scale:** Covering an area of city-like dimensions, from about 4 to 50 kilometers.
- **Regional scale:** Covering a rural area of reasonably homogeneous geography without large sources, extending from tens to hundreds of kilometers.

New monitoring stations and new monitors that are intended to be compared to the NAAQS must meet EPA siting criteria. Some sites may be appropriate for monitoring all air pollutants, while other sites may be appropriate for a particular pollutant. The District balances a wide range of pollutant siting criteria, spatial scales, monitoring objectives, and practical concerns as it plans and operates its monitoring network. Table 5 summarizes the parameters measured at each air monitoring site in the San Joaquin Valley.

## **Meteorology**

A variety of meteorological parameters are measured for various District programs affected by weather. Such programs include air quality forecasting, PAMS, exceptional events, long-term planning, and pollutant trend assessment. These activities help protect public health and have made the public and media more aware of air quality and what can be done to reduce air pollution. See Table 6 for the meteorological parameters measured in the Valley.

## **State of the Air Monitoring Network**

This air monitoring network plan summarizes the state of the District's air monitoring network during 2017. Additionally, changes that the District may initiate through December 2018 are described in the *Improvements and Planned Changes* section later in this document.



Table 5 Parameters Monitored in the San Joaquin Valley

Site Name	Ozone	PM2.5	PM10	PM10-2.5	NO2	CO	SO2	NMH	Speciated VOC	NOy	PM2.5 Speciation	Lead	Toxics	RASS*	Meteorology
Stockton–Hazelton	✓	✓	✓		✓	✓							✓		✓
Manteca		✓	✓												✓
Tracy–Airport	✓	✓	✓		✓									✓	✓
Modesto–14th St	✓	✓	✓			✓					✓				✓
Turlock	✓	✓	✓		✓										✓
Merced–Coffee	✓	✓			✓										✓
Merced–M St		✓	✓												
Madera–City	✓	✓	✓												✓
Madera–Pump Yard	✓				✓			✓	✓						✓
Tranquillity	✓	✓													✓
Fresno–Sky Park	✓				✓										✓
Clovis–Villa	✓	✓	✓		✓	✓		✓	✓						✓
Fresno–Garland	✓	✓	✓	✓	✓	✓	✓			✓	✓	✓	✓		✓
Fresno–Pacific		✓													
Fresno–Foundry					✓										✓
Fresno–Drummond	✓		✓		✓										✓
Parlier	✓				✓			✓	✓						✓
Huron		✓													✓
Hanford–Irwin	✓	✓	✓		✓										✓
Corcoran–Patterson		✓	✓												✓
Visalia–Airport														✓	✓
Visalia–Church St	✓	✓	✓		✓						✓				✓
Sequoia–Lower Kaweah	✓														✓
Sequoia–Ash Mountain	✓	✓													✓
Porterville	✓	✓													✓
Shafter	✓				✓			✓	✓						✓
Oildale	✓		✓												✓
Bakersfield–Golden / M St		✓	✓												
Bakersfield–California	✓	✓	✓		✓						✓		✓		✓
Edison	✓				✓										✓
Bakersfield–Muni	✓				✓	✓		✓	✓						✓
Bakersfield–Airport (Planz)		✓													
Arvin–Di Giorgio	✓														✓
Maricopa	✓														✓
Lebec		✓													✓

\* Radio Acoustic Sounding System (RASS)

**Table 6 San Joaquin Valley Stations Monitoring Meteorology**

Site Name	Wind Speed	Wind Direction	Outdoor Temperature	Relative Humidity	Barometric Pressure	Solar Radiation
Stockton–Hazelton	✓	✓	✓	✓		
Manteca	✓	✓	✓		✓	
Tracy–Airport	✓	✓	✓		✓	
Modesto–14th St	✓	✓	✓	✓		
Turlock	✓	✓	✓		✓	
Merced–Coffee	✓	✓	✓			
Madera–City	✓	✓	✓	✓	✓	✓
Madera–Pump Yard	✓	✓	✓	✓	✓	✓
Tranquillity	✓	✓	✓		✓	
Fresno–Sky Park	✓	✓	✓			
Clovis–Villa	✓	✓	✓	✓	✓	✓
Fresno–Garland	✓	✓	✓	✓	✓	
Fresno–Foundry	✓	✓	✓		✓	
Fresno–Drummond	✓	✓	✓		✓	
Parlier	✓	✓	✓	✓	✓	✓
Huron					✓	
Hanford–Irwin	✓	✓	✓		✓	
Corcoran–Patterson	✓	✓	✓			
Visalia–Airport	✓	✓	✓	✓	✓	✓
Visalia–Church St	✓	✓	✓	✓		
Sequoia–Lower Kaweah	✓	✓	✓	✓		✓
Sequoia–Ash Mountain	✓	✓	✓	✓		✓
Porterville	✓	✓	✓		✓	
Shafter	✓	✓	✓	✓	✓	✓
Oildale	✓	✓	✓	✓		
Bakersfield–California	✓	✓	✓	✓		
Edison	✓	✓	✓	✓		
Bakersfield–Muni	✓	✓	✓	✓	✓	✓
Arvin–Di Giorgio	✓	✓	✓	✓		
Maricopa	✓	✓	✓		✓	
Lebec	✓	✓	✓		✓	

## POLLUTANT MONITORING REQUIREMENTS

### Ozone

In 2015 EPA revised the 8-hour average ozone standard by lowering this level to 70 ppb. Ozone is formed when its precursors (oxides of nitrogen (NO<sub>x</sub>) and VOC) chemically react in the presence of heat and sunlight. The Valley's topography, high temperatures, subsidence inversions, and light winds are conducive to the formation of elevated ozone levels. Furthermore, winds (at ground level or at higher altitudes) transport pollutants from other basins into the Valley, within the Valley to areas downwind, and from the Valley into other regions.

As specified in 40 CFR part 58, Appendix D, Table D-2, ozone monitoring site requirements are based on MSA population and design values (see Table 7 below). Table 8 shows that the Valley's ozone monitoring network meets these requirements. Sites are intended to represent population exposures and maximum concentrations, so most ozone monitors are representative of neighborhood and regional scales. All of the SLAMS ozone analyzers in the District's network operate in compliance with 40 CFR Part 58 Appendix A and Appendix E and measure hourly ozone concentrations. The hourly ozone data is also used in the District's RAAN. As such, these analyzers are comparable to the ozone NAAQS and also meet the "Timely/Public" monitor objective.

**Table 7 SLAMS Minimum Ozone Monitoring Requirements**

MSA population, based on latest available census figures	Number of monitors required if:	
	Most recent 3-year design value concentrations $\geq$ 85% of any ozone NAAQS*	Most recent 3-year design value concentrations <85% of any ozone NAAQS*
> 10 million	4	2
4 – 10 million	3	1
350,000 – < 4 million	2	1
50,000 – < 350,000	1	0

\* NAAQS = 70 parts per billion (ppb)

**Table 8 Ozone Monitoring Requirements for the Valley**

MSA	2017 Population	Highest 2017 Ozone Design Value in MSA (ppb)	≥85% of 2017 ozone NAAQS*	Number of SLAMS required	SLAMS in MSA
Stockton-Lodi	746,868	77	Yes	2	2
Modesto	548,057	84	Yes	2	2
Merced	274,665	81	Yes	1	1
Madera	156,492	84	Yes	1	2
Fresno	995,975	92	Yes	2	6
Hanford–Corcoran	149,537	84	Yes	1	1
Visalia–Porterville	471,842	89	Yes	2	3
Bakersfield	760,845**	90	Yes	2	7

\*NAAQS = 70 ppb

\*\* Population estimate for Kern County (Valley Portion) was calculated using census tract data for the population living within the District's boundaries.

### Photochemical Assessment Monitoring Stations

The monitoring objective of Photochemical Assessment Monitoring Stations (PAMS) is “research support”. Federal regulations (Clean Air Act Section 182 and 40 CFR 58) require serious, severe, and extreme ozone nonattainment areas to have PAMS sites to take speciated measurements of ozone precursors and allow for better understanding of the effect of precursors, control measures, and photochemistry on ozone formation. PAMS sites measure ozone, CO, NO, NO<sub>2</sub>, NO<sub>x</sub>, and non-methane hydrocarbon (NMH) as well as meteorology. Although the Valley does not exceed federal or state standards for NO<sub>2</sub>, NO<sub>x</sub> reductions contribute to air quality improvement for both ozone and PM.

There are four classifications of PAMS:

- Type 1: **Background sites** upwind of urban areas, where ozone concentrations are presumed not to be influenced by nearby urban emissions.
- Type 2: **Maximum ozone precursor emissions sites**, typically located in an urban center, where emissions strengths are the greatest.
- Type 3: **Maximum ozone concentration sites**, intended to show the highest ozone concentrations.
- Type 4: **Downwind ozone monitoring sites**, intended to capture concentrations of transported ozone and precursor pollutants, and determine possible areas from which most of the transport may originate. Type 4 sites are currently not required for the San Joaquin Valley.

As shown in Table 9, the District has a total of six PAMS sites configured as two networks, one for the Fresno MSA and one for the Bakersfield MSA. In May 2016, the EPA approved the relocation of the ozone SLAMS monitor formerly at Arvin-Bear

Mountain to the Arvin-Di Giorgio location in Kern County. Additionally, CARB has begun the process of building a permanent shelter that should have enough space to accommodate all of the PAMS equipment intended for the site. It should be noted that, in lieu of upcoming changes to PAMS program requirements, plans to continue PAMS monitoring at Arvin are pending (see *Planned Changes/Improvements* section of this document).

Every year the PAMS program operates from June 1 through August 31 on a 1 in 3 day sampling schedule. At least four, three-hour integrated samples are collected each sampling day, which is referred to as a “Trend Day.” However, additional samples are collected on “Episode Days,” days that are forecasted to have high ozone concentrations. The goal is to sample on three to five multi-day episodes in an ozone season. PAMS equipment operates on an hourly basis year round.

**Table 9 San Joaquin Valley PAMS Network**

MSA	Site	Site Type
Fresno	Madera–Pump Yard	Type 1: Upwind/Background site
	Clovis–Villa	Type 2: Maximum precursor emissions
	Parlier	Type 3: Maximum ozone concentrations
Bakersfield	Shafter	Type 1: Upwind/Background site
	Bakersfield–Muni	Type 2: Maximum precursor emissions
	Arvin-Di Giorgio*	Type 3: Maximum ozone concentrations

\* PAMS equipment for the Type 3 site at the Arvin-Di Giorgio may be installed when space becomes available.

## Nitrogen Dioxide

In 2010, EPA retained the annual average NO<sub>2</sub> standard of 53 ppb, and established a new 1-hour NO<sub>2</sub> standard at the level of 100 ppb. Recognizing that the current NO<sub>2</sub> network is not adequate for fully assessing compliance with the new NAAQS, EPA finalized a Three-Tier Network design that will represent NO<sub>2</sub> concentrations that occur near freeways, urban areas, and locations aimed at protecting susceptible and vulnerable communities. Per 40 CFR Part 58, the Three-Tier Network design is comprised of:

- (1) One monitor that represents highest NO<sub>2</sub> exposure with a neighborhood scale or larger in CBSAs with more than 1,000,000 people.

Even though the District is not required to have an area-wide NO<sub>2</sub> monitor, the District and ARB operate an extensive NO<sub>2</sub> monitoring network consisting of 17 monitors, including one near-road NO<sub>2</sub> monitor in Fresno (with a second near-road NO<sub>2</sub> monitoring station being constructed in Bakersfield). The District locates NO<sub>2</sub> analyzers as required at PAMS sites and generally collocates NO<sub>2</sub> analyzers wherever an ozone monitor is required. Currently, all of the Valley’s

NO<sub>2</sub> monitors are in compliance with the federal NO<sub>2</sub> standards, including the Fresno near-road NO<sub>2</sub> monitoring station, which is focused on capturing peak NO<sub>2</sub> concentrations from heavily trafficked roadways. Since the Fresno near-road NO<sub>2</sub> monitoring station is well within compliance of the federal standard, it is anticipated that the Bakersfield near-road NO<sub>2</sub> monitoring station will also be in compliance.

- (2) Near-road monitoring at locations of expected maximum 1-hour NO<sub>2</sub> concentrations near heavily trafficked roads in urban areas.

On December 30, 2016, EPA finalized the revision to the Near-road NO<sub>2</sub> minimum monitoring requirements. Thus, per Section 4 of Appendix D in 40 CFR Part 58, one microscale near-road monitor is required in each CBSA with a population of 1,000,000 or more and must be located near a major road segment with a high annual average daily truck traffic (AADTT) count. An additional near-road monitor is required in CBSAs with populations of 2,500,000 or more; or in CBSAs with populations of 1,000,000 or more that have one or more road segments with 250,000 or more AADTT counts. Although the District is currently not required to have a near-road NO<sub>2</sub> monitor, it has been proactive in meeting these future requirements by already establishing a near-road NO<sub>2</sub> monitoring station in Fresno, and is working towards establishing an additional near-road station in Bakersfield, since both of these CBSAs are nearing populations of 1,000,000. The near-road air monitoring station in Fresno became operational in January 2016, and the Bakersfield near-road NO<sub>2</sub> air monitoring station is currently being built and will become operational by the beginning of 2019.

- (3) NO<sub>2</sub> network consisting of 40 monitors designed by the Regional Administrators to protect susceptible and vulnerable communities.

The third network, the Regional Administrator Required Monitoring Network (RA40) will consist of 40 NO<sub>2</sub> sites located throughout the United States and their locations will be determined by the Regional Administrators. These 40 sites would be in addition to the minimum NO<sub>2</sub> monitoring requirements. EPA Region 9 has asked the District to choose two sites for RA40 purposes. Currently, Parlier is designated as an RA40 site in the Fresno CBSA, and Bakersfield-Muni is designated as the RA40 site in the Bakersfield CBSA. These sites are located in towns with susceptible and vulnerable populations. In addition, they are downwind from urban areas.

## Carbon Monoxide

On August 12, 2011 EPA issued the decision to retain the existing NAAQS for CO. The primary standards are 9 parts per million (ppm) measured over 8 hours, and 35 ppm measured over 1 hour. Monitoring requirements for CO are specified in 40 CFR Part 58 as follows:

- CO monitors are required at all NCore sites. At least one NCore site is required in every state.

- One CO monitor is required to be placed at a near-road NO<sub>2</sub> monitoring station in a CBSA with population of 1 million or more. Moving an existing monitor to a new location is acceptable.
- EPA is providing authority to EPA Regional Administrators to require additional monitoring in case-by-case circumstances, such as in areas impacted by major stationary CO sources, in urban downtown areas, or urban street canyons, or in areas adversely impacted by meteorological and/or topographical influences.
- CO must be monitored at PAMS Type 2 sites with a trace level CO monitor.

Currently, the CBSAs within the District are comprised of less than 1 million people, thus the District is not required to place a CO monitor at a near-road NO<sub>2</sub> monitoring station. Monitoring has shown that the Valley's CO concentrations have not exceeded the NAAQS for over a decade. As noted in Section 4.2 of Appendix D of 40 CFR Part 58, there are no minimum requirements of the number of CO monitoring sites. The District and CARB continue CO monitoring to meet the requirement at its PAMS Type 2 sites and NCore site, and to supplement related meteorological and criteria pollutant data.

### Sulfur Dioxide

In 2010, EPA revised the SO<sub>2</sub> NAAQS and monitoring requirements in the Federal Register (40 CFR Part 58, Appendix D to Part 58 – Network Design Criteria of Ambient Air Quality Monitoring, Section 4.4). EPA established a new primary 1-hour standard of 75 ppb, and also revoked the previous 24-hour and annual primary standards. Under the revised SO<sub>2</sub> NAAQS, the monitoring requirements are determined by a Population Weighted Emissions Index (PWEI) value in units of million persons-tons per year. The PWEI is calculated using each CBSA's updated census data and a combined total of the latest available county level SO<sub>2</sub> emissions data in the National Emissions Inventory for the counties in each CBSA. The population of a CBSA is multiplied with the total amount of SO<sub>2</sub> in tons per year emitted within a CBSA, and the resulting product is then divided by one million to produce the PWEI value. The Valley's PWEI values are shown in Table 10.

**Table 10 Valley SO<sub>2</sub> PWEI Values for 2017**

County	Total County 2017 Population*	SO <sub>2</sub> Tons per Year**	PWEI
San Joaquin	746,868	2,044	1,527
Stanislaus	548,057	548	300
Merced	274,665	329	90
Madera	156,492	329	51
Fresno	995,975	3,687	3,672
Kings	149,537	292	44
Tulare	471,842	1,351	637
Kern	895,112	1,862	1,666

\* Population estimates are for the entire county.

\*\* SO2 Tons per Year includes the entire county. The SO2 data is the most recent data for each county from 2015.

Source: California Air Resources Board California Emission Inventory Development and Reporting System (CEIDARS) <http://www.arb.ca.gov/ei/drei/maintain/database.htm> .

As per 40 CFR Part 58, Appendix D to Part 58 – Network Design Criteria of Ambient Air Quality Monitoring, Section 4.4, at least three SO2 monitors are required in CBSAs with a PWEI value equal to or greater than 1,000,000. CBSAs with a PWEI value equal to or greater than 100,000 but less than 1,000,000, are required to have at least two SO2 monitors. A minimum of one SO2 is required in CBSAs with a PWEI value equal to or greater than 5,000, but less than 100,000.

As determined by the above Network Design Criteria PWEI, the highest PWEI value (Fresno County) is only 3,672, far below the minimum of 5,000 that would require one monitor. Incidentally, the District does not exceed the federal standard for SO2 and for CBSAs that do not exceed the federal SO2 standard there is no required number of SO2 monitors. As a result, there are no SO2 monitoring requirements for the District. Despite not having any monitoring requirements, there is one SO2 monitor operating within the District's network. This monitor is located at the Fresno-Garland AMS (Air Monitoring Station) as part of the NCore Network.

### **Reactive Nitrogen Compounds (NOy)**

Reactive Nitrogen Compounds (NOy) are among the precursors to ozone and PM2.5. As part of the National Ambient Air Monitoring Strategy (NAAMS), EPA requires NOy monitoring at 75 locations across the United States in support of a number of objectives. NCore site requirements and the PAMS program include monitoring NOy in order to meet that requirement. Measuring NOy at NCore and PAMS sites is important for understanding ozone photochemistry.

### **Toxics**

The airborne toxics program is run by CARB. Toxics measurements are collected at Stockton-Hazleton, Fresno-Garland, and Bakersfield-California. Periodic, 24-hour samples are analyzed for the following gases: benzene, carbon tetrachloride, chloroform, ethylene dibromide, ethylene dichloride, methyl chloroform, methylene chloride, perchloroethylene, toluene, trichloroethylene, and m-, p-, and o-xylene. The samples are also analyzed for 20 particulate metals including: arsenic, lead, nickel, cadmium, and hexavalent chromium.



### Detailed Site Information – Gaseous Monitors

Criteria such as monitoring methods, monitor types, spatial scales, site types, basic monitoring objectives, current sampling frequencies, and other requirements being met by the District's gaseous pollutants monitoring network are shown in Tables 11, 12, 22 through 27, and Appendix B.

**Table 11 Gaseous Monitors**

Site Name	FRM/FEM/ARM/Other				
	Ozone	NO2	CO	NMH	Speciated VOC
Stockton–Hazelton	FEM	FRM	FRM		
Tracy–Airport	FEM	FEM			
Modesto–14th St	FEM		FRM		
Turlock	FEM	FEM			
Merced–Coffee	FEM	FEM			
Madera–City	FEM				
Madera–Pump Yard	FEM	FEM		Other	Other
Tranquillity	FEM				
Fresno–Sky Park	FEM	FEM			
Clovis–Villa	FEM / FRM*	FEM	FEM	Other	Other
Fresno–Foundry		FEM			
Fresno–Drummond	FEM / FRM*	FEM			
Parlier	FEM	FEM		Other	Other
Hanford–Irwin	FEM	FEM			
Visalia–Church St	FEM	FRM			
Porterville	FEM				
Shafter	FEM	FRM		Other	Other
Oildale	FEM				
Bakersfield–California	FEM	FRM			
Edison	FEM	FRM			
Bakersfield–Muni	FEM	FEM	FEM	Other	Other
Arvin–Di Giorgio	FEM				
Maricopa	FEM				

Monitoring method information for the Fresno-Garland NCore site is provided in Table 22.

\* FEM monitor was replaced with an FRM monitor during May – June 2017.

**Table 12 Gaseous Monitors – Monitor Type**

Site Name	Monitor Type		
	Ozone	NO2	CO
Stockton–Hazelton	SLAMS	SLAMS	SLAMS
Tracy–Airport	SLAMS	SLAMS	
Modesto–14th St	SLAMS		SLAMS
Turlock	SLAMS	SLAMS	
Merced–Coffee	SLAMS	SLAMS	
Madera–City	SLAMS		
Madera–Pump Yard	SLAMS	SLAMS	
Tranquillity	SLAMS		
Fresno–Sky Park	SLAMS	SLAMS	
Clovis–Villa	SLAMS	SLAMS	SLAMS
Fresno–Foundry		SLAMS	
Fresno–Drummond	SLAMS	SLAMS	
Parlier	SLAMS	SLAMS	
Hanford–Irwin	SLAMS	SLAMS	
Visalia–Church St	SLAMS	SLAMS	
Porterville	SLAMS		
Shafter	SLAMS	SLAMS	
Oildale	SLAMS		
Bakersfield–California	SLAMS	SLAMS	
Edison	SLAMS	SLAMS	
Bakersfield–Muni	SLAMS	SLAMS	SLAMS
Arvin–Di Giorgio	SLAMS		
Maricopa	SLAMS		

Monitor type information for the Fresno-Garland NCore site is provided in Table 22.

## Particulate Matter (PM)

Particulate matter (PM) can be emitted directly as primary PM as well as formed in the atmosphere through chemical reactions of precursors to form secondary PM. Primary PM can be emitted either naturally or as a result of human (anthropogenic) activity. The resulting ambient PM mixture includes aerosols consisting of components of nitrates, sulfates, elemental carbon, organic carbon compounds, acid aerosols, trace metals, and geological materials. Under current regulations, particulate matter is differentiated by particle size as opposed to composition. Federal air quality standards differentiate two size fractions of PM: PM that is 10 microns or less in diameter (PM10) and the smaller subset that is 2.5 microns or less in diameter (PM2.5).

The mountain ranges that surround the Valley contribute to trapping pollutants, including PM, in the Valley. The Valley's frequent and strong winter temperature inversions prevent air and emissions from rising and dispersing, causing particulates to remain trapped near the surface. Prolonged periods of high pressure and stable conditions with low wind speeds can cause stagnant conditions that trap pollutants near the surface, causing PM2.5 concentrations to increase during these poor dispersion periods. During low pressure events, unstable conditions can cause vertical and horizontal mixing that help disperse PM2.5 and lower the ambient concentrations.

To better understand the influence of meteorology, natural events, and sources of emissions on the Valley's PM2.5 concentrations, the District conducted the California Regional Particulate Air Quality Study (CRPAQS). CRPAQS was a comprehensive particulate field study for which monitoring occurred between December 1999 and February 2001. Through the use of over 70 Special Purpose Monitor (SPM) PM10 sites and 50 SPM PM2.5 sites, researchers analyzed data from CRPAQS for database development, analysis, and modeling. In addition to CRPAQS, other Valley-specific air quality studies have assessed particulate emissions from agricultural operations, unpaved and paved road particulate emissions, and particulate formation in fog episodes. The design of the Valley's current PM network is an outgrowth of the results and analysis from CRPAQS and other research efforts.

The Valley's PM monitoring network includes FRM monitors, FEM monitors, and Non-FRM/FEM monitors. FRM monitors for PM are manual filter-based monitors. FRM samples are primarily collected on either a one-in-six day sampling schedule or a one-in-three day sampling schedule. FRM monitors meet the "NAAQS Comparison" objective, helping agencies determine the Valley's attainment status and helping shape the strategies for reaching or maintaining PM attainment. FRM filters can also be analyzed for PM speciation, lending to their usage for "Research Support" objectives as well.

Beta Attenuation Monitors (BAM) and Tapered Element Oscillating Microbalance (TEOM) monitors are continuous, near real-time monitors that provide the hourly PM2.5 and PM10 data used in AQI forecasts, Smoke Management System (SMS) burn allocations, hazard reduction and prescribed burning allocations and, residential wood

burning declarations. The hourly PM<sub>2.5</sub> data is also used in the District's Real-Time Air Advisory Network (RAAN). As such, these monitors help meet the "Timely/Public" objective.

Not all real-time monitors meet the "NAAQS Comparison" objective because they do not meet the rigorous engineering design, quality assurance, and quality control standards necessary for comparison to the NAAQS. An FEM monitor is often a real-time monitor that has been designated by EPA as being equivalent to FRM monitors. FEMs satisfy both the "NAAQS Comparison" objective and the "Timely/Public" objective. All of the Valley's TEOMs are FEMs, and some of the Valley's BAMs are FEMs.

Several PM<sub>2.5</sub> analyzers within the District's network are located at sites that are not required by EPA. The District operates these sites for various reasons, including complying with state laws (Huron), as a settlement to a lawsuit (Tracy-Airport), and for the purposes of helping the District's RAAN and forecasting programs (Porterville and Lebec, where the Lebec site was donated to the District). Additionally, settlements of California Environmental Quality Act (CEQA) lawsuits between a private company and a private citizen required the company to give the District specific air monitoring equipment to be operated at specific sites. All of these sites and/or equipment are not required for NAAQS purposes.

The District operates four PM<sub>2.5</sub> analyzers (parameter code 88502) as SPMs. These analyzers have not been certified by EPA as comparable to the PM<sub>2.5</sub> NAAQS and do not meet all of the certification requirements. Specifically, EPA requires a runtime of 42 minutes per hour with an eight-minute count and these analyzers operate with a runtime of 50 minutes per hour with a four-minute count. Additionally, these instruments use a Sharp Cut Cyclone PM<sub>2.5</sub> inlet instead of a Very Sharp Cut Cyclone PM<sub>2.5</sub> inlet. Finally, some of these analyzers do not support the approved software to operate in a manner comparable to the NAAQS. While these sites are non-FEMs, they produce valuable data that is of sufficient quality for their intended purposes. All other required PM<sub>2.5</sub> analyzers in the District's network, both SLAMS and SPM, are operated in compliance with 40 CFR Part 58 Appendix A and Appendix E, and are comparable to the PM<sub>2.5</sub> NAAQS.

### **Detailed Site Information – PM Monitors**

As mentioned above, monitoring sites and monitors must meet siting and operational criteria as outlined in 40 CFR Part 58. Criteria such as monitor types, spatial scales, site types, basic monitoring objectives, current sampling frequencies, and other requirements being met by the District's PM network are shown in Tables 19 through 28 and Appendix B.

## **PM Collocation Requirements**

Per 40 CFR 58 Appendix A, Sections 3.2.5 and 3.2.6, the District's Particulate Matter collocation requirements are met by the Primary Quality Assurance Organization (PQAO). CARB is the PQAO for the District as well as several other air districts. See CARB's Air Monitoring Network Plans for details on how collocation requirements are met by the PQAO. Table 21 shows the collocated PM monitors currently operating in the District's monitoring network.

## **Public Review of Changes to the PM<sub>2.5</sub> Monitoring Network**

Public input is required whenever the District proposes to move an existing violating PM<sub>2.5</sub> monitor (40 CFR 58.10(c)). The District uses the annual Air Monitoring Network Plan to notify and seek public comment on any planned changes to the existing PM<sub>2.5</sub> network. The public is provided 30 days to comment on the Air Monitoring Network Plan and any PM<sub>2.5</sub> network changes. The plan is regularly posted on the District website, after which the public is notified of the availability of the document for the 30-day review. In the event of unanticipated changes to the PM<sub>2.5</sub> network that occur outside the Air Monitoring Network Plan process, the District will post the required documentation on its website and seek public comment.

## **PM<sub>10</sub> Monitoring Requirements**

The San Joaquin Valley has been redesignated to attainment for PM<sub>10</sub>, and the District's *2007 PM<sub>10</sub> Maintenance Plan* and ongoing PM<sub>10</sub> monitoring will assure continued compliance with the federal standard. All required PM<sub>10</sub> analyzers, both SLAMS and SPM, are operated in compliance with 40 CFR Part 58 Appendix A and Appendix E, and are comparable to the PM<sub>10</sub> NAAQS which is 150 µg/m<sup>3</sup>.

As shown in Table 13 below, Table D-4 of Appendix D to Part 58 specifies that the minimum number of PM<sub>10</sub> sites required per MSA is based on population. As such, Table 14 shows that the District's PM<sub>10</sub> monitoring network meets the requirements for the San Joaquin Valley. Additionally, the year 2017 24-hour PM<sub>10</sub> highest concentrations for each PM<sub>10</sub> monitoring site in the District's network are provided in Table 15.

**Table 13 Minimum PM10 Monitoring Requirements\***

Population category	High concentration**	Medium concentration***	Low concentration****
>1,000,000	6-10	4-8	2-4
500,000-1,000,000	4-8	2-4	1-2
250,000-500,000	3-4	1-2	0-1
100,000-250,000	1-2	0-1	0

\* A range is presented, and the actual number of stations per area is jointly determined by EPA, CARB, and the local agency.

\*\* High concentration areas are those for which ambient PM10 data show ambient concentrations exceeding the PM10 NAAQS by 20 percent or more.

\*\*\* Medium concentration areas are those for which ambient PM10 data show ambient concentrations exceeding 80 percent of the PM10 NAAQS.

\*\*\*\* Low concentration areas are those for which ambient PM10 data show ambient concentrations less than 80 percent of the PM10 NAAQS. These minimum monitoring requirements apply in the absence of a design value.

**Table 14 PM10 Monitoring Requirements for the Valley**

MSA	County	2017 Population	PM10		
			24-hour 2017 Highest concentration in MSA ( $\mu\text{g}/\text{m}^3$ )*	Number of SLAMS required	SLAMS in MSA
Stockton-Lodi	San Joaquin	746,868	151	2 – 4	3
Modesto	Stanislaus	548,057	129	2 – 4	2
Merced	Merced	274,665	146	1 – 2	1
Madera	Madera	156,492	149	0 – 1	1
Fresno	Fresno	995,975	154	2 – 4	3
Hanford–Corcoran	Kings	149,537	154	0 – 1	2
Visalia–Porterville	Tulare	471,842	144	1 – 2	1
Bakersfield**	Kern	760,845	149	2 – 4	3

\* Exceptional Events are not included.

\*\* Population estimate for Kern County (Valley Portion) was calculated using census tract data for the population living within the District's boundaries.

**Table 15 24-Hour PM10 highest concentrations at each site\***

MSA	Site Name	2017 Highest Concentration**
Stockton-Lodi	Stockton-Hazelton	89
	Manteca	106
	Tracy-Airport	151
Modesto	Modesto-14th St	129
	Turlock	111
Merced	Merced-M St	146
Madera	Madera-City	149
Fresno	Fresno-Garland***	154
	Fresno-Drummond	115
	Clovis-Villa	134
Hanford-Corcoran	Hanford-Irwin	154
	Corcoran-Patterson	150
Visalia-Porterville	Visalia-Church St	144
Bakersfield	Oildale	149
	Bakersfield-Golden State/M St	109
	Bakersfield-California	138

\* Exceptional Events are not included. Current Sampling Frequency information is provided in Table 27.

\*\* Current Sampling Frequency information for the Fresno-Garland NCore site is provided in Table 22.

\*\*\* Highest concentrations obtained from AQS AMP450NC and AMP350 Reports. The concentrations for some sites require further calculation due to data incompleteness.

## PM2.5 Monitoring Requirements

The San Joaquin Valley is designated nonattainment for PM2.5. Per 40 CFR Part 58 Appendix D Table D-5 the minimum number of PM2.5 sites required per MSA is based on population (see Table 16). Table 17 shows that the District's PM2.5 monitoring network meets the PM2.5 monitoring requirements for the San Joaquin Valley. Additionally, the 2015 – 2017 24-hour PM2.5 and annual design values for each site in the District's PM2.5 network are provided in Table 18.

**Table 16 Minimum PM2.5 Monitoring Requirements**

MSA population	Most recent 3-year design value $\geq 85\%$ of the 24-Hour or the Annual PM2.5 NAAQS*	Most recent 3-year design value $< 85\%$ of the 24-Hour or the Annual PM2.5 NAAQS**(*)
>1,000,000	3	2
500,000-1,000,000	2	1
50,000-<500,000	1	0

\* 24-hour PM<sub>2.5</sub> NAAQS is 35  $\mu\text{g}/\text{m}^3$ . The Annual PM2.5 NAAQS is 12  $\mu\text{g}/\text{m}^3$ .

\*\* These minimum monitoring requirements apply in the absence of a design value.

**Table 17 PM2.5 Monitoring Requirements for the Valley\***

MSA	County	2017 Population	PM2.5				
			24-hour 2015-2017 Design Value in MSA ( $\mu\text{g}/\text{m}^3$ )	Annual 2015-2017 Design Value in MSA ( $\mu\text{g}/\text{m}^3$ )	Number of SLAMS required	Number of SLAMS in MSA	Number of Continuous PM2.5 Monitors in MSA**
Stockton-Lodi	San Joaquin	746,868	39	12.2	2	2	3
Modesto	Stanislaus	548,057	45	13.2	2	2	2
Merced	Merced	274,665	39	12.7	1	2	1
Madera	Madera	156,492	42	12.8	1	1	1
Fresno***	Fresno	995,975	54	14.0	2	4	6
Hanford-Corcoran****	Kings	149,537	54	16.4	1	2	2
Visalia-Porterville	Tulare	471,842	54	15.7	1	1	2
Bakersfield*****	Kern	760,845	59	17.3	2	3	2

- \* Air quality data may include data influenced by exceptional events and/or data completeness and substitution requirements.
- \*\* Number of continuous monitors includes regulatory and non-regulatory monitors.
- \*\*\* The PM2.5 FRM monitor at Fresno-Garland is one of the monitors helping meet the number of PM2.5 SLAMS required in the Fresno MSA.
- \*\*\*\* Hanford design values are displayed for the Hanford-Corcoran MSA. Corcoran 2015-17 design values are not representative of ambient concentrations due to incomplete data in 2015 resulting from the shelter being destroyed in a fire.
- \*\*\*\*\* Population estimate for Kern County (Valley Portion) was calculated using census tract data for the population living within the District's boundaries.



**Table 18 24-Hour and Annual PM<sub>2.5</sub> Maximum Design Values**

MSA	Site Name	2015-2017 24-Hour Design Value	2015-2017 Annual Design Value	Max Site in MSA	
				24-Hour	Annual
Stockton-Lodi	Stockton–Hazelton	39	12.2	✓	✓
	Manteca	36	11.2		
Modesto	Modesto–14th St*	39	--		
	Turlock	45	13.2	✓	✓
Merced	Merced–M St	38	12.1		
	Merced-Coffee	39	12.7	✓	✓
Madera	Madera–City	42	12.8	✓	✓
Fresno	Tranquility	32	8.7		
	Clovis–Villa	46	13.6		
	Fresno–Pacific	52	14.0		
	Fresno-Garland	54	14.0	✓	✓
Hanford-Corcoran	Corcoran–Patterson*	--	--		
	Hanford–Irwin	54	16.4	✓	✓
Visalia-Porterville	Visalia–Church St	54	15.7	✓	✓
Bakersfield	Bakersfield–Golden / M St	58	15.9		
	Bakersfield–California	59	15.7		
	Bakersfield–Airport (Planz)	59	17.3	✓	✓

\* 24-hour and annual design values are not displayed for Corcoran and Modesto-14<sup>th</sup> St due data incompleteness, which caused concentrations to be unrepresentative of ambient conditions.

### PM<sub>2.5</sub> Chemical Speciation Site Requirements

Per CFR 40 Part 58, the Chemical Speciation Network (CSN) includes Speciation Trends Network stations (STN) and supplemental speciation stations that provide chemical species data of fine particulate. Each State must conduct chemical speciation monitoring and analysis at sites that have been designated part of the STN and approved by the Administrator. Monitoring methods and sampling schedules used at the PM<sub>2.5</sub> chemical speciation urban trends sites must be approved by the Administrator. Additionally, the sites must also include analysis for elements, selected anions and cations, and carbon. Speciation data can be used to support a variety of efforts including:

- Air quality modeling analyses to help track NAAQS attainment progress and emissions controls.
- Aiding the interpretation of health studies by linking health effects to PM2.5 constituents.
- Understanding the effects of atmospheric elements on visibility.
- Assisting with air monitoring network design and siting adjustments.

In addition to the STN requirement, EPA encourages air agencies to operate additional supplemental speciation monitors to meet needs independent of the requirement such as supporting health effects related studies, and developing SIPs. There are seven PM2.5 speciation monitors operating in the District's network. Four (along with two collocated) of the monitors that meet the STN requirement, and two that are supplemental monitors. Details on these PM2.5 speciation monitors are shown in Table 19, and Appendix B.

**Table 19 PM2.5 Speciation Monitors**

Site Name	Network Affiliation	Monitor Type	FRM/FEM/ARM/Other	Site Type	Spatial Scale	Basic Monitoring Objective	Current Sampling Frequency	QA Collocated
Modesto–14th St	CSN Supplemental	SLAMS	Other	PE	N	RS	1:6	
Fresno-Garland*	NCore, STN	Other	Other	PE	N,U	RS	1:3	
	NCore, STN	Other	Other	PE	N,U	RS	1:3	
Visalia–Church St	CSN Supplemental	SLAMS	FRM	PE	N	RS	1:3	
	STN	SLAMS	Other	PE	N,U	RS	1:3	
Bakersfield–California	CSN, STN	Other	Other	PE	N,U	RS	1:3	
	CSN, STN	Other	Other	PE	N,U	RS	1:6	✓**

PE – Population Exposure N – Neighborhood U – Urban RS – Research TP – Timely/Public  
 Hourly = One sample every hour 1:3 = 1 in 3 day sampling 1:6 = 1 in 6 day sampling QA = Quality Assurance  
 \* PM2.5 Speciation monitor information for the Fresno-Garland NCore site is also provided in Table 22.  
 \*\* Two collocated monitors operating.

Per network plan requirements described above, Tables 20 and 21 show the types of monitoring methods, collocated monitors, and monitor types operating in the District's PM monitoring network.

Table 20 PM Monitors

Site Name	FRM/FEM/ARM/Other						QA Collocated			
	PM10 (man.)	PM10 (cont.)	PM2.5 (man.)	PM2.5 (cont.)	Valid PM2.5 Design Value? Yes or No		PM10 (man.)	PM10 (cont.)	PM2.5 (man.)	PM2.5 (cont.)
					24-Hour NAAQS	Annual NAAQS				
Stockton– Hazelton	FRM			FEM	Yes	Yes				FEM
Manteca		FEM		FEM	Yes	Yes				FEM
Tracy–Airport		FEM		Non–FEM						
Modesto– 14th St		FEM		FEM	Yes	No			FRM	
Turlock	FRM			FEM	Yes	Yes				
Merced– Coffee				FEM	Yes	Yes				
Merced–M St	FRM		FRM		Yes	Yes				
Madera–City		FEM		FEM	Yes	Yes			FRM	
Tranquillity				FEM	Yes	Yes				
Clovis–Villa	FRM	FEM		FEM	Yes	Yes			FRM	
Fresno– Pacific			FRM		Yes	Yes				
Fresno– Drummond	FRM						FRM			
Huron				Non–FEM						
Corcoran– Patterson		FEM	FRM	FEM	No	No				
Hanford– Irwin	FRM	FEM		FEM	Yes	Yes				
Visalia– Church St		FEM	FRM	Non-FEM						
Porterville				Non-FEM						
Oildale	FRM	FEM								
Bakersfield– Golden / M St	FRM		FRM		Yes	Yes				
Bakersfield– California	FRM		FRM	Non–FEM			FRM		FRM	
Bakersfield– Airport (Planz)			FRM		Yes	Yes				
Lebec				Non–FEM						

cont. – Continuous man. – Manual QA = Quality Assurance

Monitoring method and monitor collocation information for the Fresno-Garland NCore site is provided in Table 22.

Table 21 PM Monitors – Monitor Type

Site Name	Monitor Type				QA Collocated			
	PM2.5 (man.)	PM2.5 (cont.)	PM10 (man.)	PM10 (cont.)	PM2.5 (man.)	PM2.5 (cont.)	PM10 (man.)	PM10 (cont.)
Stockton–Hazelton		SLAMS	SLAMS			SLAMS *		
Manteca		SLAMS		SLAMS		SLAMS		
Tracy–Airport		SPM		SLAMS				
Modesto–14th St		SLAMS		SLAMS	SLAMS			
Turlock		SLAMS	SLAMS					
Merced–Coffee		SLAMS						
Merced–M St	SLAMS		SLAMS					
Madera–City		SLAMS		SLAMS	SLAMS			
Tranquillity		SLAMS						
Clovis–Villa	SLAMS	SLAMS	SLAMS	SLAMS		SLAMS		
Fresno–Pacific	SLAMS							
Fresno–Drummond			SLAMS				SLAMS	
Huron		SPM						
Corcoran–Patterson	SLAMS	SLAMS		SLAMS				
Hanford–Irwin		SLAMS	SLAMS	SLAMS				
Visalia–Church St	SLAMS	OTHER		SLAMS				
Porterville		SPM						
Oildale	SLAMS		SLAMS					
Bakersfield–Golden / M St	SLAMS		SLAMS					
Bakersfield–California	SLAMS	OTHER	SLAMS		SLAMS		SLAMS	
Bakersfield–Airport (Planz)	SLAMS							
Lebec		SPM						

cont. – Continuous man. – Manual QA = Quality Assurance

Monitor information for the Fresno-Garland NCore site is provided in Table 22.

\* Per update from ARB, this QA Collocated PM2.5 monitor is being reclassified as a SLAMS monitor.

## Lead

Per the revised lead NAAQS and monitoring requirements which became effective on January 26, 2011, EPA requires monitoring agencies to install non-source oriented lead monitors at NCore sites in CBSAs with populations of 500,000 or greater. The Fresno-Garland air monitoring site (an NCore site) is the only site within the District's network that meets these criteria. In December 2011, CARB began measuring lead at the Fresno-Garland site to satisfy this requirement. EPA also requires state monitoring agencies to use the emission threshold of 0.5 tons per year (tpy) when determining if a monitor should be placed near an industrial facility that emits lead. The emission threshold for airport sources is 1.0 tpy, except for airports that are included in special studies. The District has not identified any lead sources above the aforementioned thresholds, thus it is not required to monitor for that threshold at this time.

## NCore

On October 17, 2006, EPA issued final amendments to the ambient air monitoring requirements for criteria pollutants. These amendments were codified in Title 40 CFR parts 53 and 58 and established a requirement for NCore multi-pollutant monitoring stations to be operational by January 1, 2011. Since ARB's Fresno-First site already met many of the NCore requirements for filter-based and continuous PM<sub>2.5</sub>, speciated PM<sub>2.5</sub>, ozone, and meteorological monitoring, CARB submitted an NCore monitoring plan to the EPA in November 2009. The ARB's Fresno-First site was selected by EPA to be an NCore site for the Fresno, CA MSA. In December 2010, CARB installed trace level CO, trace level SO<sub>2</sub>, trace level NO<sub>y</sub>, and continuous PM<sub>10-2.5</sub> monitors at this site. A gas dilution calibrator, a zero air generator, and digital data loggers were also installed to support NCore monitoring. In December 2011, CARB installed a TSP-lead sampler which completed all the pollutant monitoring requirements for the NCore program. In January 2012, CARB relocated the Fresno-First site (AQS #: 06-019-0008) two blocks north to the Fresno-Garland site (AQS #: 06-019-0011). The Fresno-Garland site continues to serve as the NCore site for the Fresno, CA MSA. Table 22 shows the different parameters measured at the NCore site.

**Table 22 Fresno-Garland NCore Site**

Pollutant	Monitor Type	FRM/FEM/ARM/Other	Site Type	Spatial Scale	Basic Monitoring Objective	Current Sampling Frequency	QA Collocation
Ozone	SLAMS	FEM	PE	U	NC,RS	Hourly	
NO <sub>2</sub>	SLAMS	FRM	Max PEI	U	NC,RS	Hourly	
CO	SLAMS	FRM	PE	U	NC,RS	Hourly	
SO <sub>2</sub>	SLAMS	FEM	PE	U	NC,RS	Hourly	
NO <sub>y</sub>	SLAMS	Other	PE	U	NC,RS	Hourly	
Toxics	SLAMS	Other	PE	N	RS,TP	Hourly	
PM <sub>2.5</sub> (man.)	SLAMS	FRM	HC	N	NC,RS	1:1	
PM <sub>2.5</sub> (man.)	SLAMS	FRM	HC,PE,QA	N	NC,RS	1:6	✓
PM <sub>2.5</sub> (cont.)	SLAMS	FEM	HC,QA	N	NC,RS	Hourly	✓
PM <sub>2.5</sub> Speciation (STN)	Other	Other	PE	N,U	RS	1:3	
	Other	Other	PE	N,U	RS	1:3	
PM <sub>10</sub> STP (cont.)	SLAMS	FEM	PE	N	NC,RS	Hourly	
PM <sub>10</sub> STP (Lead TSP) (man.)	SLAMS	Other	PE	N	NC	1:6	
PM <sub>10</sub> LC (Lead TSP) (man.)	SLAMS	FEM	PE	N	NC,RS,TP	1:6	
PM <sub>10-2.5</sub> (cont.)	SLAMS	FEM	PE,QA	N	NC,RS	Hourly	✓ *

cont. – Continuous    man. – Manual    PE – Population Exposure    HC – Highest Concentration  
 N – Neighborhood    U – Urban    RS – Research    MxPEI – Max Precursor Emissions Impact  
 NC – NAAQS Comparison    TP – Timely/Public    STP – Standard Temperature and Pressure  
 Hourly = One sample every hour    1:1 = One sample per day    1:6 = 1 in 6 day sampling

\* Serving as primary monitor

### Non-EPA Federal Monitors

Within the District's air monitoring network are Non-EPA Federal monitors which are located in Sequoia and Kings Canyon National Park and operated by the National Forest Service. The monitors operating at the Sequoia-Ash Mountain AMS are affiliated with specific networks, the Clean Air Status and Trends Network (CASTNET) and the Interagency Monitoring of Protected Visual Environments (IMPROVE) network. CASTNET assesses trends in pollutant concentrations, atmospheric deposition, and ecological effects due to changes in air pollutant emissions. The IMPROVE network monitors PM in order to characterize all of the major components and many trace constituents of the particulate matter that impair visibility in Federal Class I Areas such as national parks, national wilderness areas, and national monuments. Details on these monitors are shown in Table 23 and Appendix B.

**Table 23 Non-EPA Federal Monitors**

<b>Sequoia–Ash Mountain</b>						
<b>Parameter</b>	<b>Site Type</b>	<b>FRM/FEM/ARM/Other</b>	<b>Spatial Scale</b>	<b>Network affiliation</b>	<b>Basic Monitoring Objective</b>	<b>Current Sampling Frequency</b>
Ozone	HC, RT	Other	R	CASTNET	NC, RS, TP	Hourly
PM2.5 (continuous)	RT	FEM	R	IMPROVE	RS, TP	Hourly
Meteorology	GB	Other	R	CASTNET	RS, TP	Hourly
<b>Sequoia–Lower Kaweah</b>						
<b>Parameter</b>	<b>Site Type</b>	<b>FRM/FEM/ARM/Other</b>	<b>Spatial Scale</b>	<b>Network affiliation</b>	<b>Basic Monitoring Objective</b>	<b>Current Sampling Frequency</b>
Ozone	RT	Other	R	None	NC, RS, TP	Hourly
Meteorology	GB	Other	R	None	RS, TP	Hourly

HC – High Concentration RT - Regional Transport GB – General Background R - Regional  
 NC – NAAQS Comparison RS – Research TP – Timely/Public Hourly = One sample every hour  
 CASTNET – Clear Air Status and Trends Network

As previously noted, purpose, siting, and operational requirements for each monitor must be met as outlined in Appendices A, C, D, and E of 40 CFR Part 58. Accordingly, this detailed site information is provided in Tables 24 through 28 as well as in Appendix B of this network plan.

**Table 24 SLAMS – Site Type**

<b>Site Name</b>	<b>Ozone</b>	<b>PM2.5 (man.)</b>	<b>PM2.5 (cont.)</b>	<b>PM10 (man.)</b>	<b>PM10 (cont.)</b>	<b>NO2</b>	<b>CO</b>	<b>NMH</b>
Stockton–Hazelton	HC, PE		HC, PE	HC		PE	PE	
Manteca			PE		PE			
Tracy–Airport	RT				RT	RT		
Modesto–14th St	HC, PE	PE, QA	PE		PE		PE	
Turlock	HC, PE		HC, PE	PE		PE		
Merced–Coffee	HC, PE		PE			PE		
Merced–M St		HC, PE		HC, PE				
Madera–City	HC, GB	HC, QA	PE		PE			
Madera–Pump Yard	HC, GB					PE		PE
Tranquillity	PE		PE					
Fresno–Sky Park	HC, PE, RT					PE		
Clovis–Villa	Max PEI, HC	HC	HC	PE	HC	HC	Max PEI, PE	HC
Fresno–Pacific		PE						
Fresno–Foundry						HC		
Fresno–Drummond	HC, PE, RT			PE, QA		HC		

**Table 24 SLAMS – Site Type (continued)**

Site Name	Ozone	PM2.5 (man.)	PM2.5 (cont.)	PM10 (man.)	PM10 (cont.)	NO2	CO	NMH
Parlier	HC, RT					PE		PE
Corcoran–Patterson		HC	HC, PE		HC, PE			
Hanford–Irwin	HC, PE		PE	PE	PE	PE		
Visalia–Church St	GB	HC, PE	RT, PE		PE	PE		
Porterville	HC, PE		PE					
Shafter	GB, PE					PE		PE
Oildale	HC, RT			SO	SO			
Bakersfield–Golden / M St		PE		PE				
Bakersfield–California	HC, GB	HC, PE	PE	PE		PE		
Edison	HC, RT					PE		
Bakersfield–Muni	HC					HC	PE	PE
Bakersfield–Airport (Planz)		HC, PE						
Arvin–Di Giorgio	HC, PE							
Maricopa	HC, RT							

cont. – Continuous man. – Manual PE – Population Exposure HC – Highest Concentration  
 RT – Regional Transport GB – General/Background QA – QA Collocation SO – Source Oriented  
 Site Type information for the Fresno-Garland NCore site is provided in Table 22.

**Table 25 SLAMS – Spatial Scale**

Site	Ozone	PM2.5 (man.)	PM2.5 (cont.)	PM10 (man.)	PM10 (cont.)	NO2	CO	NMH
Stockton–Hazelton	N		N	N		N	N	
Manteca			N		N			
Tracy–Airport	R				R	R		
Modesto–14th St	N	N	N		N		N	
Turlock	N		N	N		N		
Merced–Coffee	N		N			N		
Merced–M St		N		N				
Madera–City	N	N	N		N			
Madera–Pump Yard	N					N		N
Tranquillity	U		U					
Fresno–Sky Park	N					N		
Clovis–Villa	N	N	N	N	N	N	N	N



**Table 25 SLAMS – Spatial Scale (continued)**

Site	Ozone	PM2.5 (man.)	PM2.5 (cont.)	PM10 (man.)	PM10 (cont.)	NO2	CO	NMH
Fresno–Pacific		N						
Fresno–Foundry						MC		
Fresno–Drummond	N			N		N		
Parlier	N					N		N
Corcoran–Patterson		N			N			
Hanford–Irwin	N		N	N	N	N		
Visalia–Church St	N	N	N		N	N		
Porterville	N		N					
Shafter	N					N		N
Oildale	U			MD				
Bakersfield– Golden / M St		MC		MC				
Bakersfield–California	N	N	N	N		N		
Edison	N					N		
Bakersfield–Muni	N					N	N	N
Bakersfield–Airport (Planz)		N						
Arvin–Di Giorgio	N							
Maricopa	N							

N – Neighborhood U – Urban R – Regional MC – Microscale MD – Middle scale  
cont. – Continuous man. – Manual

Spatial Scale information for the Fresno-Garland NCore site is provided in Table 22.

**Table 26 SLAMS – Basic Monitoring Objective**

Site	Ozone	PM2.5 (man.)	PM2.5 (cont.)	PM10 (man.)	PM10 (cont.)	NO2	CO	NMH
Stockton– Hazelton	NC, RS, TP		NC, RS, TP	NC, RS		NC, RS, TP	NC, RS, TP	
Manteca			NC,RS,TP		NC,RS,TP			
Tracy–Airport	NC,RS,TP				NC,RS,TP	NC, RS, TP		
Modesto– 14th St	NC,RS,TP	NC, RS	NC,RS,TP		NC,RS,TP		NC, RS, TP	
Turlock	NC,RS,TP		NC,RS,TP	NC,RS		NC, RS, TP		
Merced– Coffee	NC,RS,TP		NC,RS,TP			NC, RS,TP		
Merced–M St		NC, RS		NC RS				
Madera–City	NC,RS,TP	NC,RS	NC,RS,TP		NC,RS,TP			
Madera– Pump Yard	NC,RS,TP					NC, RS, TP		RS
Tranquillity	NC,RS,TP		NC,RS,TP					
Fresno–Sky Park	NC,RS,TP					NC, RS, TP		
Clovis–Villa	NC,RS,TP	NC,RS	NC,RS,TP	NC,RS	NC,RS,TP	NC, RS, TP	NC, RS, TP	RS

**Table 26 SLAMS – Basic Monitoring Objective (continued)**

Site	Ozone	PM2.5 (man.)	PM2.5 (cont.)	PM10 (man.)	PM10 (cont.)	NO2	CO	NMH
Fresno–Pacific		NC,RS						
Fresno–Foundry						NC,RS,TP		
Fresno–Drummond	NC,RS,TP			NC,RS		NC		
Parlier	NC,RS,TP					NC,RS,TP		RS
Corcoran–Patterson		NC,RS	NC,RS,TP		NC,RS,TP			
Hanford–Irwin	NC,RS,TP		NC,RS,TP	NC,RS	NC,RS,TP	NC,RS,TP		
Visalia–Church St	NC,RS,TP	NC,RS	RS,TP		NC,RS,TP	NC,RS,TP		
Porterville	NC,RS,TP							
Shafter	NC,RS,TP					NC,RS,TP		RS
Oildale	NC,RS,TP			NC,RS	NC,RS,TP			
Bakersfield–Golden / M St		NC,RS		NC,RS				
Bakersfield–California	NC,RS,TP	NC,RS	RS,TP	NC,RS		NC,RS,TP		
Edison	NC,RS,TP					NC,RS,TP		
Bakersfield–Muni	NC,RS,TP					NC,RS,TP	NC,RS,TP	RS
Bakersfield–Airport (Planz)		NC,RS						
Arvin–Di Giorgio	NC,RS,TP							
Maricopa	NC,RS,TP							

NC – NAAQS Comparison RS – Research TP – Timely/Public cont. – Continuous man. – Manual  
 Basic Monitor Objective information for the Fresno-Garland NCore site is provided in Table 22.

**Table 27 SLAMS – Current Sampling Frequency**

Site Name	Ozone	PM2.5 (man.)	PM2.5 (cont.)	PM10 (man.)	PM10 (cont.)	NO2	CO	NMH
Stockton–Hazelton	Hourly		Hourly	1:6		Hourly	Hourly	
Manteca			Hourly		Hourly			
Tracy–Airport	Hourly				Hourly	Hourly		
Modesto–14th St	Hourly	1:12	Hourly		Hourly		Hourly	
Turlock	Hourly		Hourly	1:6		Hourly		
Merced–Coffee	Hourly		Hourly			Hourly		
Merced–M St		1:3		1:6				
Madera–City	Hourly	1:12	Hourly		Hourly			
Madera–Pump Yard	Hourly					Hourly		Hourly
Tranquillity	Hourly		Hourly					

**Table 27 SLAMS – Current Sampling Frequency (continued)**

Site Name	Ozone	PM2.5 (man.)	PM2.5 (cont.)	PM10 (man.)	PM10 (cont.)	NO2	CO	NMH
Fresno–Sky Park	Hourly					Hourly		
Clovis–Villa	Hourly	1:3	Hourly	1:6	Hourly	Hourly	Hourly	Hourly
Fresno–Pacific		1:3						
Fresno–Foundry						Hourly		
Fresno–Drummond	Hourly			1:6		Hourly		
Parlier	Hourly					Hourly		Hourly
Corcoran–Patterson		1:3	Hourly		Hourly			
Hanford–Irwin	Hourly		Hourly	1:6	Hourly	Hourly		
Visalia–Church St	Hourly	1:3	Hourly		Hourly	Hourly		
Porterville	Hourly							
Shafter	Hourly					Hourly		Hourly
Oildale	Hourly			1:6				
Bakersfield–Golden / M St		1:3		1:6				
Bakersfield–California	Hourly	1:1	Hourly	1:6		Hourly		
Edison	Hourly					Hourly		
Bakersfield–Muni	Hourly					Hourly	Hourly	Hourly
Bakersfield–Airport (Planz)		1:3						
Arvin–Di Giorgio	Hourly							
Maricopa	Hourly							

cont. – Continuous    man. – Manual    Hourly = One sample every hour    1:1 = One sample per day

1:3 = 1 in 3 day sampling    1:6 = 1 in 6 day sampling

Current Sampling Frequency information for the Fresno-Garland NCore site is provided in Table 22.

**Table 27 SPM (PM2.5 Continuous)**

Site Name	Site Type	Spatial Scale	Basic Monitoring Objective	Current Sampling Schedule
Tracy–Airport	RT	R	TP	Hourly
Huron	PE	N	TP	Hourly
Porterville	PE	N	TP	Hourly
Lebec	PE	N	TP	Hourly

PE – Population Exposure    RT – Regional Transport    N – Neighborhood    R – Regional    Timely/Public

Hourly = One sample every hour

## **IMPROVEMENTS AND PLANNED CHANGES TO THE DISTRICT'S AIR MONITORING NETWORK**

The Valley air monitoring network is continually being improved. MSA/CBSA-specific changes are generally described below. Before any action is taken on the planned changes noted in this section, the District will work with CARB and EPA, as appropriate, to address necessary requirements for documentation. A summary of the planned changes to the District's air monitoring network during 2017/2018 is provided in Table 28.

### **Network Changes during 2017/2018**

#### **Deployment of New Air Monitoring Network Technology**

During this last year, the District continued its deployment of Teledyne 602 instrument into its air monitoring network, which measures both PM10 and PM2.5 simultaneously and in real-time, allowing for more efficient monitoring operations. The Teledyne 602 units that are currently operating have been deployed to the air monitoring sites of Manteca, Madera-City, Clovis, Corcoran, and Hanford. The District has additionally deployed new EPA approved NOx and ozone samplers with improved technology as they have become available, improving the accuracy of these measurements throughout the air monitoring network. To allow for staff to complete calibration work remotely and enhance the calibration process, the District has also deployed new calibration units to sites measuring gas parameters through the network.

### **Planned Improvements and Other Changes Scheduled for 2018/2019**

#### **Arvin-Di Giorgio PAMS Type 3 Station**

The District is required to have a PAMS Type 3 air monitoring station in the Bakersfield MSA. The District has not been operating a PAMS Type 3 station since the Arvin-Bear Mountain site closed. A permanent air monitoring shelter of sufficient size to house the equipment may soon be built at Arvin-Di Giorgio due to EPA's recent approval of CARB's relocation request<sup>1</sup>. Once this construction is complete, the District may install PAMS Type 3 equipment to begin PAMS monitoring again in the Arvin area (see discussion below). However, this change is dependent on how the PAMS network may be structured in the future, as discussed below.

#### **PAMS Network Design**

EPA recently changed the monitoring requirements for areas currently required to operate and maintain PAMS networks. Under these changes, PAMS monitoring will be required at NCore sites in an area's network, which is the Fresno-Garland site for the

---

<sup>1</sup> Kurpius, Meredith. Letter to CARB. 2 May. 2016. TS

San Joaquin Valley, and will be optional at sites currently measuring PAMS parameters, as defined in this network plan. These changes are designated to become effective in 2019 for affected areas. The District will work closely with ARB and EPA to ensure that active and informative PAMS monitoring is conducted moving forward, particularly given the District's ongoing efforts toward attaining the federal ozone standards.

### **Lower Air Profilers**

As a part of the upcoming changes to PAMS monitoring requirements, the operation of lower air profilers (LAP) will no longer be required in PAMS networks. The District currently operates two LAPs in support of the PAMS program, those being at the Tracy and Visalia-Airport air monitoring sites. Although the information the LAPs provided has been useful for air quality forecasting and modeling purposes, their operation and maintenance has proven to be cost prohibitive and burdensome. As an alternative, the District may invest in other measurement equipment that will provide similar information, but at a much lower cost.

### **Visalia-Airport Site**

The Visalia-Airport site in Tulare County currently only measures meteorology as well as parameters measured by the LAP on site. Since the Visalia-Airport site exists primarily to support the PAMS program through the operation of its LAP, should the LAP be discontinued as discussed above, the District may also consider closing down the site in its entirety as it will no longer be required for the PAMS network or the network as a whole. Since meteorology is already measured at the Visalia airport itself and at the nearby Visalia-Church air monitoring site, the data being collected could be considered redundant in nature. Should the District proceed with a plan to close the site, we will work closely with ARB and EPA through this process.

### **Fresno-Sierra Sky Park Site**

Vegetation to the south and southwest of the Fresno-Sierra Sky Park site has grown to the point of disrupting wind flow from the south, southwest and the southeast. In addition, the construction of new homes has encroached upon the perimeter of the site causing potential obstructions. Based on these conditions, the site is no longer meeting the EPA's siting requirements for SLAMS monitors. The District has made efforts to resolve the landscaping issues with adjacent landowners, but has been unsuccessful in gaining cooperation for the needed changes to the landscaping. In the meantime, the District will continue to operate the site as is and apply in the EPA AQS database the qualifier flag 'SX' (which means 'Does not meet siting criteria') to all gaseous data going forward to let users of the data know there are siting issues and to use the data with caution. The District will continue to make efforts to resolve the siting issues with adjacent land owners and evaluate other potential options for this site.

**Stockton-Hazelton Site**

Within this next year, ARB plans to replace the FRM PM10 Hi-Vol unit with an FEM PM10 BAM unit. This change is planned to occur by the end of 2018.

**Progress report on Bakersfield Near-Road NO2 site**

At this time, the District meets or exceeds all near-road NO2 requirements. The District is being proactive by building a second near-road NO2 site in the Bakersfield CBSA long before it is required considering the population growth rate. Construction of Bakersfield near-road NO2 site has started and is planned to be operational by the beginning of 2019. This planned site is located just north of Truxton Avenue on the east side of Highway 99.

**All other Sites**

No other changes are proposed at this time to any other sites in the District.

**Table 28 Summary of Proposed Changes to the Air Monitoring Network**

<b>CBSA: Stockton</b>		<b>County: San Joaquin</b>	
<b>Site Name</b>	<b>Operating Agency</b>	<b>Planned Changes</b>	
Stockton–Hazelton	CARB	None	
Manteca	SJVAPCD	None	
Tracy–Airport	SJVAPCD	Potential LAP closure	
<b>CBSA: Modesto</b>		<b>County: Stanislaus</b>	
<b>Site Name</b>	<b>Operating Agency</b>	<b>Planned Changes</b>	
Modesto–14th St	CARB	None	
Turlock	SJVAPCD	None	
<b>CBSA: Merced</b>		<b>County: Merced</b>	
<b>Site Name</b>	<b>Operating Agency</b>	<b>Planned Changes</b>	
Merced–Coffee	SJVAPCD	None	
Merced–M St	SJVAPCD	None	
<b>CBSA: Madera</b>		<b>County: Madera</b>	
<b>Site Name</b>	<b>Operating Agency</b>	<b>Planned Changes</b>	
Madera–City	SJVAPCD	None	
Madera–Pump Yard	SJVAPCD	None	
<b>CBSA: Fresno</b>		<b>County: Fresno</b>	
<b>Site Name</b>	<b>Operating Agency</b>	<b>Planned Changes</b>	
Tranquillity	SJVAPCD	None	
Fresno–Sky Park	SJVAPCD	None	
Clovis–Villa	SJVAPCD	None	
Fresno–Garland	CARB	None	
Fresno–Drummond	SJVAPCD	None	
Fresno–Pacific	SJVAPCD	None	
Fresno–Foundry (near-road)	SJVAPCD	None	
Parlier	SJVAPCD	None	
<b>CBSA: Kings</b>		<b>County: Kings</b>	
<b>Site Name</b>	<b>Operating Agency</b>	<b>Planned Changes</b>	
Hanford–Irwin	SJVAPCD	None	
Corcoran–Patterson	SJVAPCD	None	

**Table 32 Summary of Proposed Changes to the Air Monitoring Network (cont'd)**

<b>CBSA: Visalia–Porterville</b>		<b>County: Tulare</b>	
<b>Site Name</b>	<b>Operating Agency</b>	<b>Planned Changes</b>	
Visalia–Airport	SJVAPCD	Potential LAP and site closure	
Visalia–Church St	CARB	None	
Sequoia–Lower Kaweah	NPS	None	
Sequoia–Ash Mountain	NPS	None	
Porterville	SJVAPCD	None	
<b>CBSA: Bakersfield</b>		<b>County: Kern (Valley Portion Only)</b>	
<b>Site Name</b>	<b>Operating Agency</b>	<b>Planned Changes</b>	
Shafter	Shared	None	
Oildale	CARB	None	
Arvin–Di Giorgio	CARB	A permanent air monitoring shelter may soon be built since EPA approved CARB's relocation request for monitoring in Arvin.	
Bakersfield–California	CARB	None	
Bakersfield–Golden State/M St	SJVAPCD	None	
Bakersfield–Westwind (near-road)	SJVAPCD	Construction of this site has started and should become operational by January 2018	
Bakersfield–Muni	SJVAPCD	None	
Bakersfield–Airport (Planz)	CARB	None	
Edison	CARB	None	
Maricopa	SJVAPCD	None	
Lebec	SJVAPCD	None	



## DATA SUBMISSION REQUIREMENTS

Air Quality and Precision data are required to be submitted to EPA 90 days after the end of the calendar quarter once all air quality assurance checks are completed. Accuracy data is submitted to EPA by CARB as part of their scheduled audits. CARB is responsible for certifying data from all CARB-operated air monitoring sites, as well as weighing and certifying filter-based measurements from District operated sites. The measurements are weighed at CARB's laboratory in Sacramento, CA. For information on CARB's data certification, see CARB's air monitoring network plan at <http://www.arb.ca.gov/aqd/amnr/amnr.htm>. The District is responsible for certifying data from all District-operated air monitoring sites. **The District certified the 2017 data on April 26, 2018.**

**ACRONYMS AND ABBREVIATIONS**

AIRS:	Aerometric Information Retrieval System
AQI:	Air Quality Index
AQS:	Air Quality System
CARB:	California Air Resources Board
ARM:	Approved Regional Method
BAM:	Beta Attenuation Monitor
CAA:	Clean Air Act
CASTNET:	Clean Air Status and Trends Network
CBSA:	Core-Based Statistical Area
CCOS:	Central California Ozone Study
CFR:	Code of Federal Regulations
CRPAQS:	California Regional Particulate Air Quality Study
CO:	Carbon Monoxide
CO <sub>2</sub> :	Carbon Dioxide
CSA:	Combined statistical area
District:	San Joaquin Valley Air Pollution Control District
EBAM:	Environmental Beta Attenuation Monitor
EPA:	U.S. Environmental Protection Agency
FEM:	Federal Equivalent Method
FIPS:	Federal information processing standard
FR:	Federal Register
FRM:	Federal Reference Method
GHG:	Green House Gases
IMPROVE:	Interagency Monitoring of Protected Visual Environments
LAP:	Lower Air Profiler
MSA:	Metropolitan statistical area
NAAQS:	National Ambient Air Quality Standard
NCore:	National Core
NMH:	Non-Methane Hydrocarbons
NO <sub>2</sub> :	Nitrogen Dioxide
NOAA:	National Oceanic and Atmospheric Administration
NO <sub>x</sub> :	Oxides of Nitrogen
NO <sub>y</sub> :	Reactive Nitrogen
NPS:	National Park Service
O <sub>3</sub> :	Ozone
PAMS:	Photochemical Assessment Monitoring Station
Pb:	Lead
PM:	Particulate Matter
PM <sub>2.5</sub> :	Particulate Matter 2.5 microns or less in diameter
PM <sub>10</sub> :	Particulate Matter 10 microns or less in diameter
SLAMS:	State and Local Air Monitoring Station
SJV:	San Joaquin Valley
SJVAPCD:	San Joaquin Valley Air Pollution Control District
SMS:	Smoke Management System
SO <sub>2</sub> :	Sulfur Dioxide
SPM:	Special Purpose Monitor
STN:	Speciated Trends Network
TEOM:	Tapered Element Oscillating Microbalance
TSP:	Total Suspended Particles
Valley:	San Joaquin Valley
VOC:	Volatile Organic Compounds

This page is intentionally blank.

**APPENDIX A:**  
**Air Monitoring Site Descriptions**


This page is intentionally blank.

**Stockton-Hazelton**

The Stockton-Hazelton monitoring site is operated by CARB and is located in the Stockton, CA metropolitan area. It began operating in January 1976. The purpose of the site is to monitor representative concentrations of ozone, PM2.5, and PM10 in an urban area. The site also monitors CO, NO2, toxics, and meteorology.

Site name:	Stockton-Hazelton
AQS ID:	06-077-1002
County:	San Joaquin
Street Address:	1601 E Hazelton St, Stockton CA 95205
Geographic Coordinates:	37.9507 N, -121.2689 W
Distance to road (meters):	62 m (north)
Traffic Count (AADT; Year):	4,000; 2014*
Ground Cover:	Paved
Representative Statistical Area (CBSA):	Stockton-Lodi

\*Traffic count estimated by City of Stockton Public Works Traffic Engineering Division

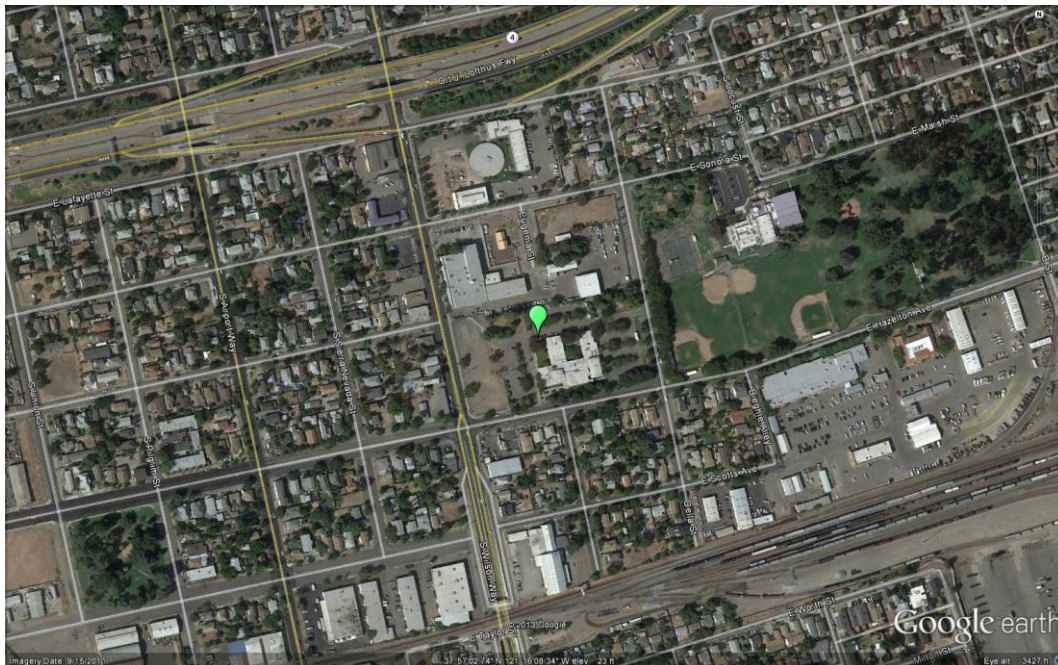


**Manteca**

The Manteca monitoring site is located in Manteca, CA and operated by SJVAPCD. It became operational in November 2010. The purpose of the site is to monitor representative concentrations of PM2.5 and PM10 from upwind and nearby urban areas. The site also monitors meteorology.

Site name:	Manteca
AQS ID:	06-077-2010
County:	San Joaquin
Street Address:	530 Fishback Rd, Manteca CA 95337
Geographic Coordinates:	37.7933 N, -121.2477 W
Distance to road (meters):	12 m (west)
Traffic Count (AADT; Year):	13,383; 2014*
Ground Cover:	Paved, vegetative
Representative Statistical Area (CBSA):	Stockton-Lodi

\*Traffic count for nearest roads: Yosemite Ave and Airport Way. Source: TJKM Transportation Consultants

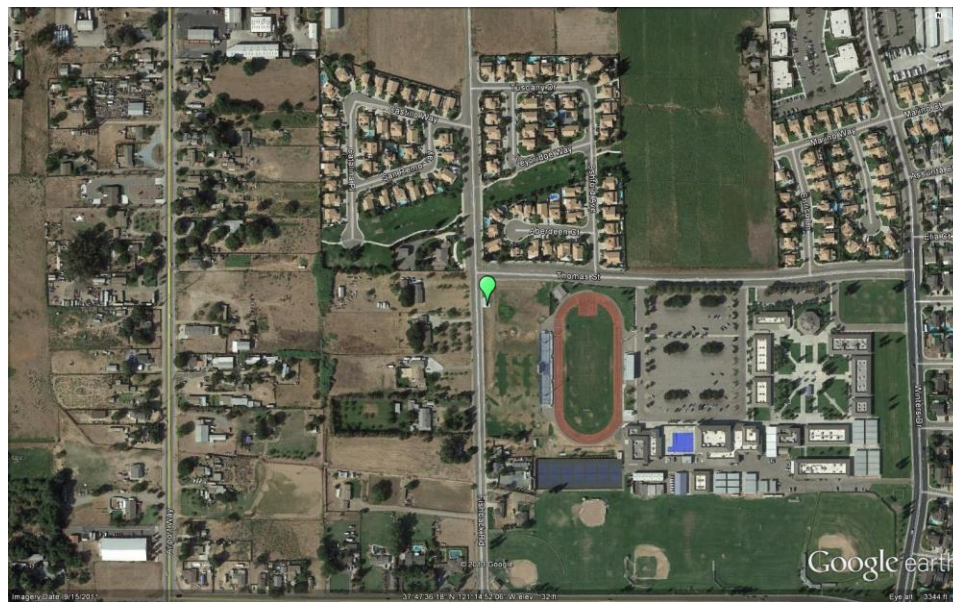


## Tracy-Airport

The Tracy-Airport monitoring site, located in Tracy, CA, was part of a settlement from a lawsuit between the District and CARB that took place in 1995. This air monitoring station was installed for the purpose of monitoring transport of air pollution from the Bay Area to the San Joaquin Valley. The site became operational in 1994 and was operated by CARB until June 1995. The District began operating the site in 1996. The site has been moved several times over the years and became operational at its current location in January 2006. The site monitors transport of ozone, NO<sub>2</sub>, PM<sub>2.5</sub>, and PM<sub>10</sub> from upwind and nearby urban areas. The site also measures meteorology.

Site name:	Tracy-Airport
AQS ID:	06-077-3005
County:	San Joaquin
Street Address:	5749 S Tracy Blvd, Tracy CA 95376
Geographic Coordinates:	37.6826 N, -121.4423 W
Distance to road (meters):	700 m (east)
Traffic Count (AADT; Year):	4,063; 2014*
Ground Cover:	Dirt and Gravel
Representative Statistical Area (CBSA):	Stockton-Lodi

\*Traffic count for nearest roads: Linne Rd, Corral Hollow Rd. Source: TJKM Transportation Consultants

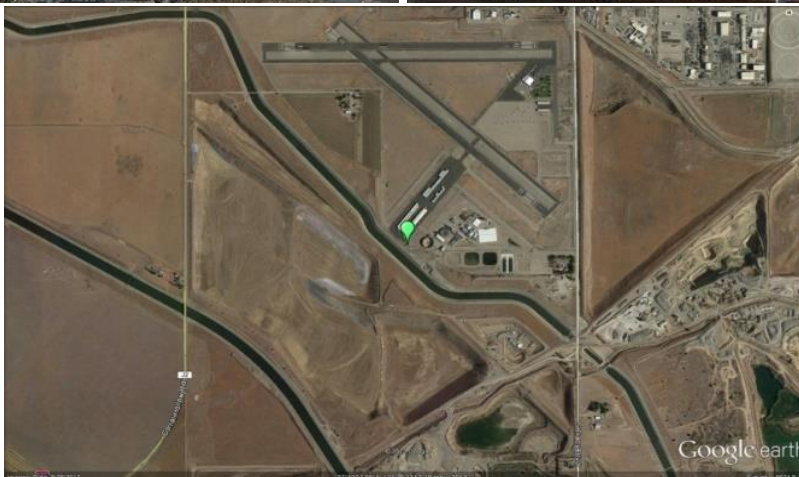





## Modesto-14<sup>th</sup> St

The Modesto-14<sup>th</sup> St monitoring site is operated by CARB and is located in the Modesto, CA metropolitan area. It began operating in January 1981. The purpose of the site is to monitor representative concentrations of ozone, PM<sub>2.5</sub>, and PM<sub>10</sub> in local and upwind urban areas. The site also monitors CO, PM<sub>2.5</sub> Speciation, and meteorology.

Site name:	Modesto-14 <sup>th</sup> St
AQS ID:	06-099-0005
County:	Stanislaus
Street Address:	814 14th St, Modesto CA 95354
Geographic Coordinates:	37.6421 N, -120.9942 W
Distance to road (meters):	50 m (southwest)
Traffic Count (AADT; Year):	122,000; 2014*
Ground Cover:	Paved
Representative Statistical Area (CBSA):	Modesto

\* Traffic count for nearest roads: H Street / CA Route 99. Source: Caltrans 2016 AADT

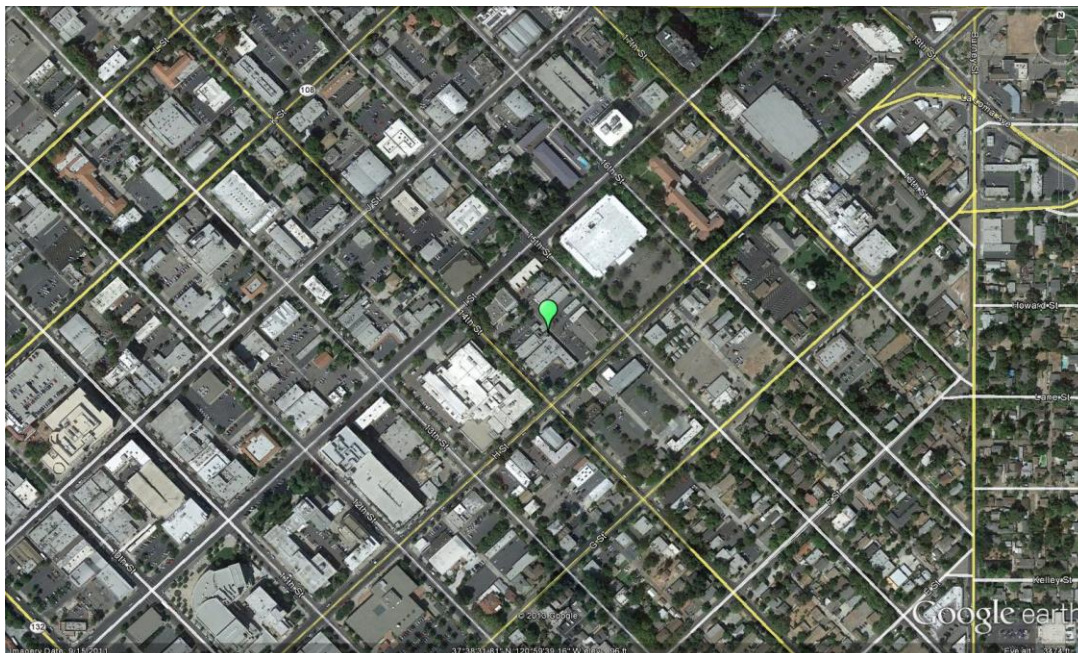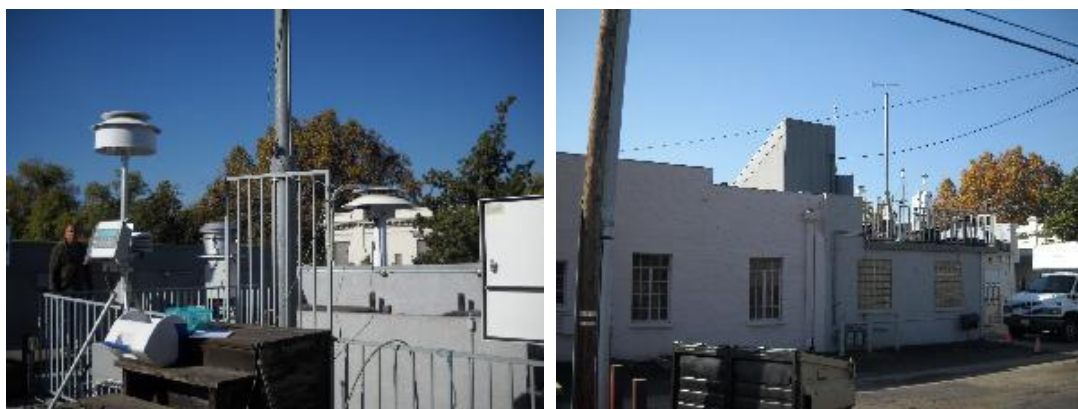


**Turlock**

The Turlock monitoring site is operated by SJVAPCD and is located in Turlock, CA. It began operating in April 1992. The purpose of the site is to monitor representative concentrations of ozone, PM2.5, and PM10 from upwind urban areas. The site also monitors NO2, and meteorology.

Site name:	Turlock
AQS ID:	06-099-0006
County:	Stanislaus
Street Address:	900 S Minaret St., Turlock CA 95380
Geographic Coordinates:	37.4880 N, -120.8360 W
Distance to road (meters):	40 m (northeast)
Traffic Count (AADT; Year):	7,186; 2015*
Ground Cover:	Gravel
Representative Statistical Area (CBSA):	Modesto

\* Minaret St/East F St near Golden State Blvd. Source: City of Turlock Engineering Division 2015

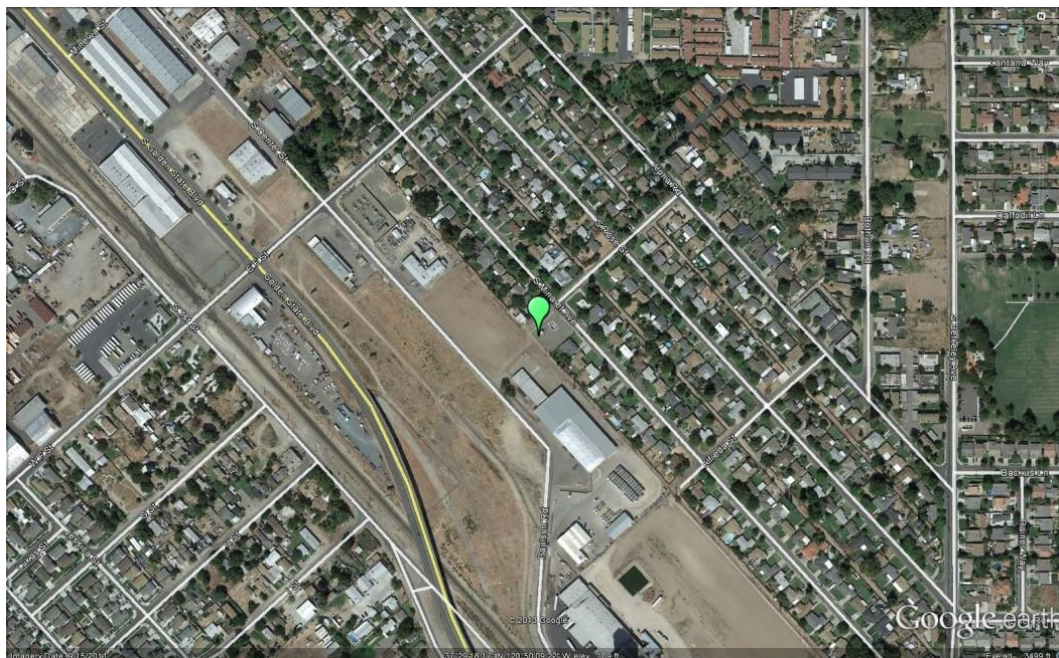


**Merced-M St**

The Merced-M St monitoring site is operated by SJVAPCD and is located in Merced, CA. It began operating in April 1999. The purpose of the site is to monitor representative concentrations of PM2.5 and PM10 responses from upwind urban areas.

Site name:	Merced-M St
AQS ID:	06-047-2510
County:	Merced
Street Address:	2334 M St, Merced CA 95340
Geographic Coordinates:	37.3086 N, -120.4800 W
Distance to road (meters):	55 m (northwest)
Traffic Count (AADT; Year):	51,000; 2014*
Ground Cover:	Paved, gravel
Representative Statistical Area (CBSA):	Merced

\*Traffic count for nearest roads: R St / CA Route 99. Source: Caltrans 2016 AADT

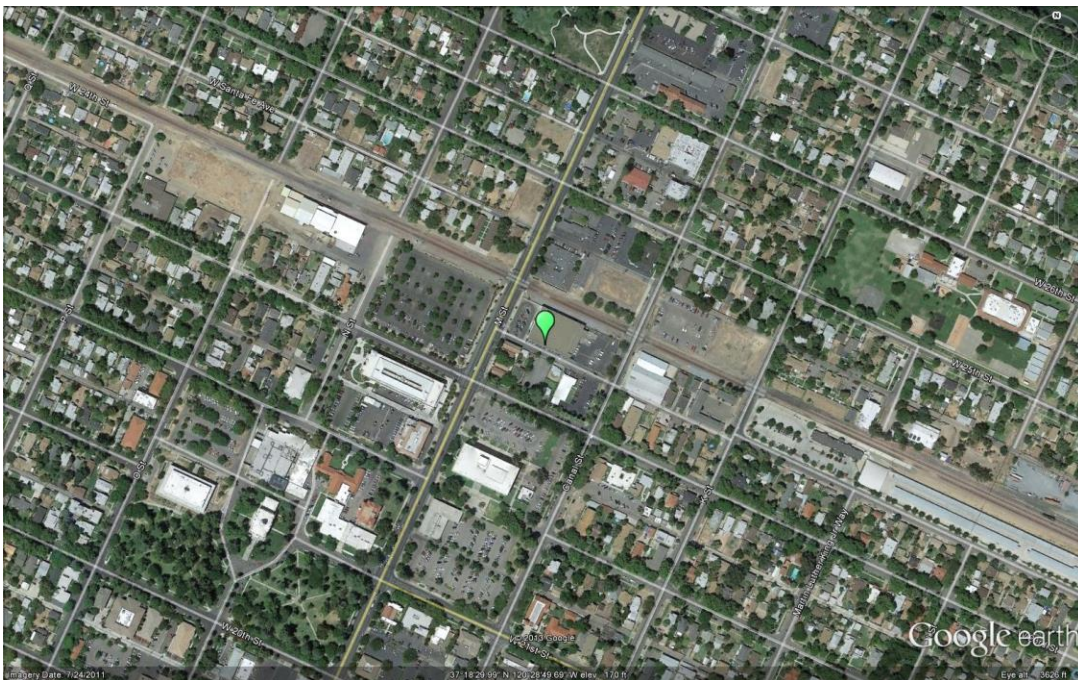


**Merced-Coffee**

The Merced-Coffee monitoring site is operated by SJVAPCD and is located in the Merced, CA. It began operating in October 1991. The purpose of the site is to monitor representative concentrations of ozone and PM2.5 responses from upwind urban areas. The site also monitors NO2 and meteorology.

Site name:	Merced-Coffee
AQS ID:	06-047-0003
County:	Merced
Street Address:	385 S. Coffee St., Merced CA 95340
Geographic Coordinates:	37.2816 N, -120.4340 W
Distance to road (meters):	15 m (east)
Traffic Count (AAD; Year):	42,500; 2014*
Ground Cover:	Vegetative, dirt and gravel
Representative Statistical Area (CBSA):	Merced

\*Traffic count for nearest roads: Childs Ave / CA Route 99. Source: Caltrans 2016 AADT

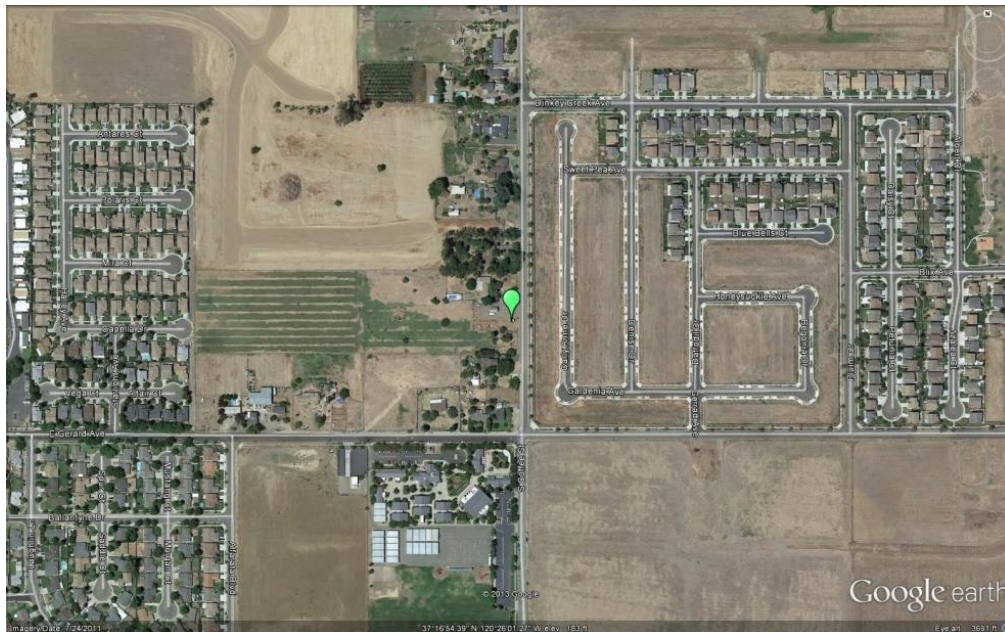


**Madera-City**

The Madera-City monitoring site is operated by SJVAPCD and is located in the city of Madera, CA. It began operating in June 2010. The purpose of the site is to monitor representative concentrations of ozone, PM2.5, PM10. The site also monitors meteorology.

Site name:	Madera-City
AQS ID:	06-039-2010
County:	Madera
Street Address:	28261 Avenue 14, Madera CA 93638
Geographic Coordinates:	36.9532 N, -120.0342 W
Distance to road (meters):	70 m (south)
Traffic Count (AADT; Year):	386; 2017*
Ground Cover:	Paved, dirt, and vegetative
Representative Statistical Area (CBSA):	Madera

\*Traffic count for nearest roads: Avenue14 west of Road 29, westbound trips per hour in 24 hours. Source: Madera County Transportation Commission 2017 Traffic Volumes Report.

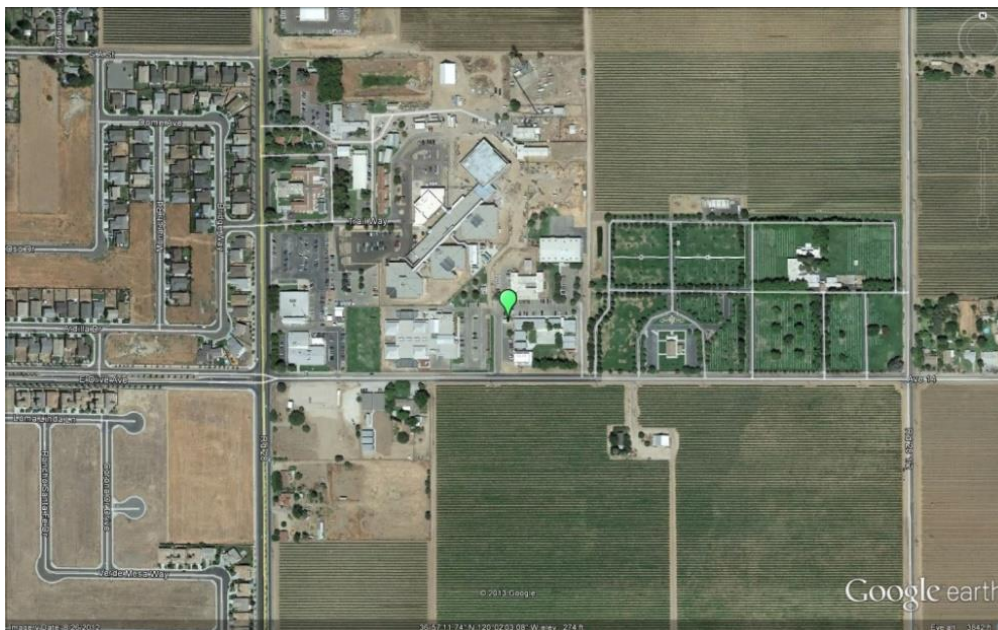

## Madera-Pump Yard

The Madera-Pump Yard monitoring site is operated by SJVAPCD and is located in southern Madera County. It began operating in July 1997. This site was established as a PAMS Type 1 site, and located in an area upwind of Fresno essentially void of upwind or local ozone precursor emissions influences. This site monitors ozone, NO<sub>2</sub>, NMH, Speciated-VOC, and meteorology for the PAMS program.

Site name:	Madera-Pump Yard
AQS ID:	06-039-0004
County:	Madera
Street Address:	Avenue 8 and Road 29 1/2, Madera CA 93637
Geographic Coordinates:	36.867125 N, -120.010158 W
Distance to road (meters):	20 m (west)
Traffic Count (AADT; Year):	2,980; 2017*
Ground Cover:	Dirt, paved
Representative Statistical Area (CBSA):	Madera

\*Traffic count for nearest roads: Avenue 7 west of CA Route 99, westbound trips per hour in 24 hours. Source: Madera County Transportation Commission 2017 Traffic Volumes Report.




### Tranquillity

The Tranquillity monitoring site is located in western Fresno County. It began operating in September 2009 and is operated by SJVAPCD. The purpose of this site is to monitor representative background and rural pollutant concentrations of ozone and PM2.5. The site also monitors meteorology.

Site name:	Tranquillity
AQS ID:	06-019-2009
County:	Fresno
Street Address:	32650 W Adams, Tranquillity CA 93668
Geographic Coordinates:	36.6008 N, -120.3822 W
Distance to road (meters):	200 m (south)
Traffic Count (AADT; Year):	2,292; 2018*
Ground Cover:	Dirt, vegetative
Representative Statistical Area (CBSA):	Fresno

\* Raw traffic count for nearest roads: Northbound Derrick Ave between W Nebraska Ave and West Mountain View Ave

Source: Fresno COG Traffic Counts, 2007-2018 Kittelson & Associates, Inc.

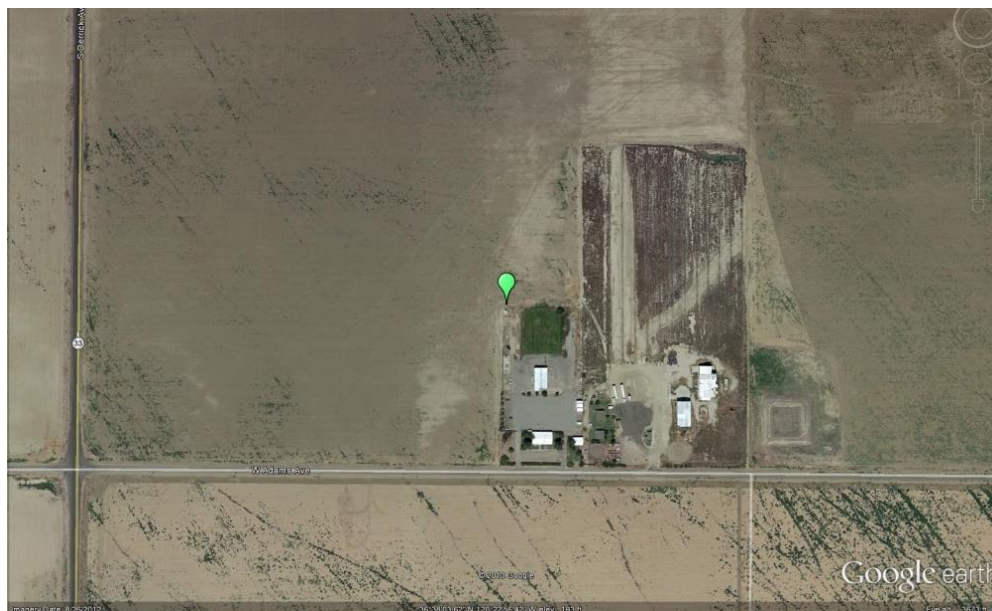


### Fresno-Sierra Sky Park

The Fresno-Sierra Sky Park monitoring site is operated by SJVAPCD and is located in the Fresno, CA metropolitan area. It began operating in July 1986. The purpose of the site is to monitor representative concentrations of ozone responses in an urban area. In addition to ozone, the site also monitors NO2 and meteorology.

Site name:	Fresno-Sky Park
AQS ID:	06-019-0242
County:	Fresno
Street Address:	4508 Chennault Ave, Fresno CA 93722
Geographic Coordinates:	36.8405 N, -119.8740 W
Distance to road (meters):	12 m (west)
Traffic Count (AADT; Year):	15,626; 2018*
Ground Cover:	Gravel, dirt
Representative Statistical Area (CBSA):	Fresno

\*Raw traffic count in a 24-hour period for nearest roads: Spruce Ave east of Milburn Ave  
 Source: Fresno COG Traffic Counts, 2007-2018 Kittelson & Associates, Inc.

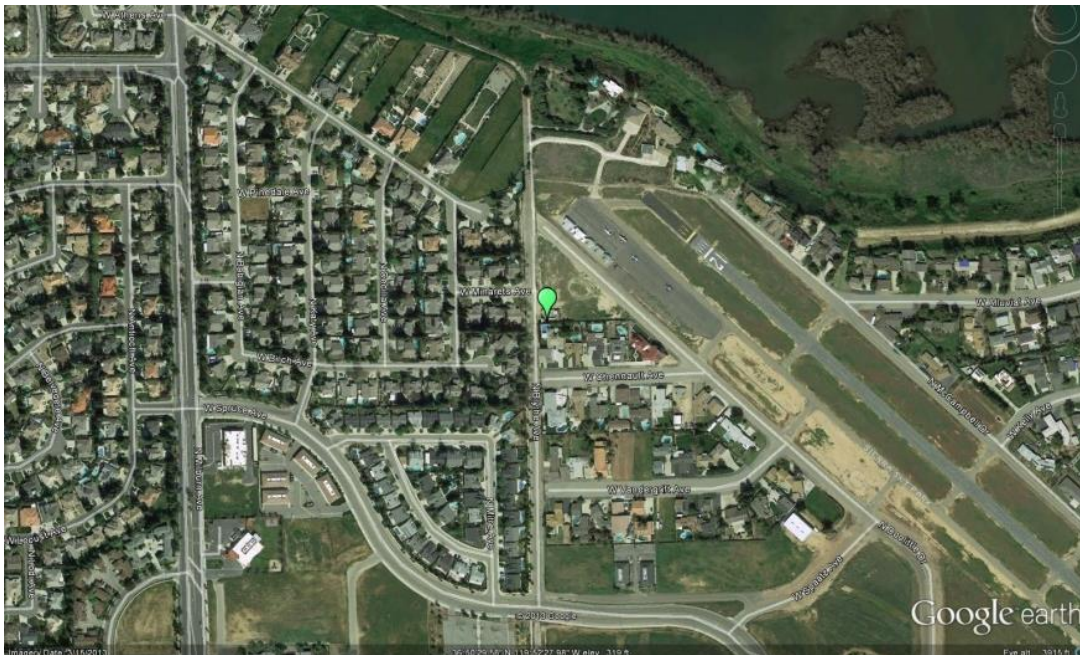




**Clovis-Villa**

The Clovis-Villa monitoring site is operated by SJVAPCD and is located in the northeastern portion of the Fresno, CA metropolitan area. It began operating in September 1990. This site is a PAMS Type 2 site, a site intended to measure maximum ozone precursor emissions. The site monitors ozone, CO, NO<sub>2</sub>, NMH and speciated-VOC, and meteorology for the PAMS program. PM<sub>2.5</sub> and PM<sub>10</sub> are also monitored at the site.

Site name:	Clovis-Villa
AQS ID:	06-019-5001
County:	Fresno
Street Address:	908 N Villa Ave, Clovis CA 93612
Geographic Coordinates:	36.8194 N, -119.7160 W
Distance to road (meters):	260 m (east)
Traffic Count (AADT; Year):	13,890; 2008*
Ground Cover:	Paved
Representative Statistical Area (CBSA):	Fresno

\*Raw traffic count in a 24-hour period: Eastbound Bullard Ave/Villa Ave intersection, Source: Fresno COG Fresno County Regional Traffic Monitoring Report 2013 (latest available)

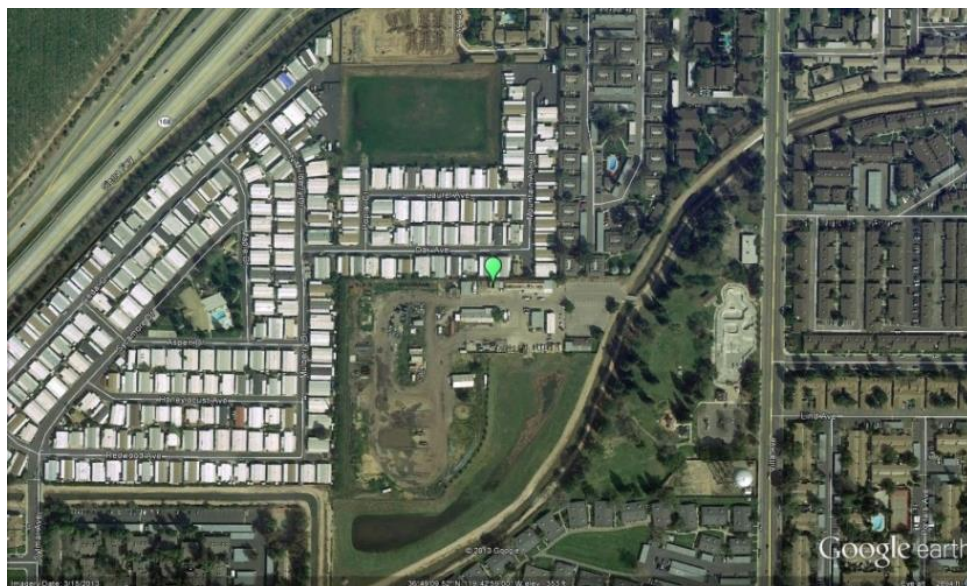


**Fresno-Garland**

The Fresno-Garland monitoring site is a National Core (NCore) site operated by CARB and is located in the Fresno, CA metropolitan area. It began operating in December 2011. The purpose of the site is to monitor representative concentrations of ozone, PM2.5, and PM10 in an urban area. The site also monitors PM10-2.5, PM2.5 Speciation, CO, NO2, NOy, SO2, Lead, Toxics, and meteorology.

Site name:	Fresno–Garland
AQS ID:	06-019-0011
County:	Fresno
Street Address:	3727 N. First St., Ste.104, Fresno CA 93726
Geographic Coordinates:	36.7853 N, -119.7732 W
Distance to road (meters):	30 m (south)
Traffic Count (AADT; Year):	7,460; 2011*
Ground Cover:	Gravel covered tar paper with wooden deck walkways
Representative Statistical Area (CBSA):	Fresno

\*Raw traffic count in a 24-hour period for nearest roads: First St near Dakota Ave  
 Source: Fresno COG Fresno County Regional Traffic Monitoring Report 2013.

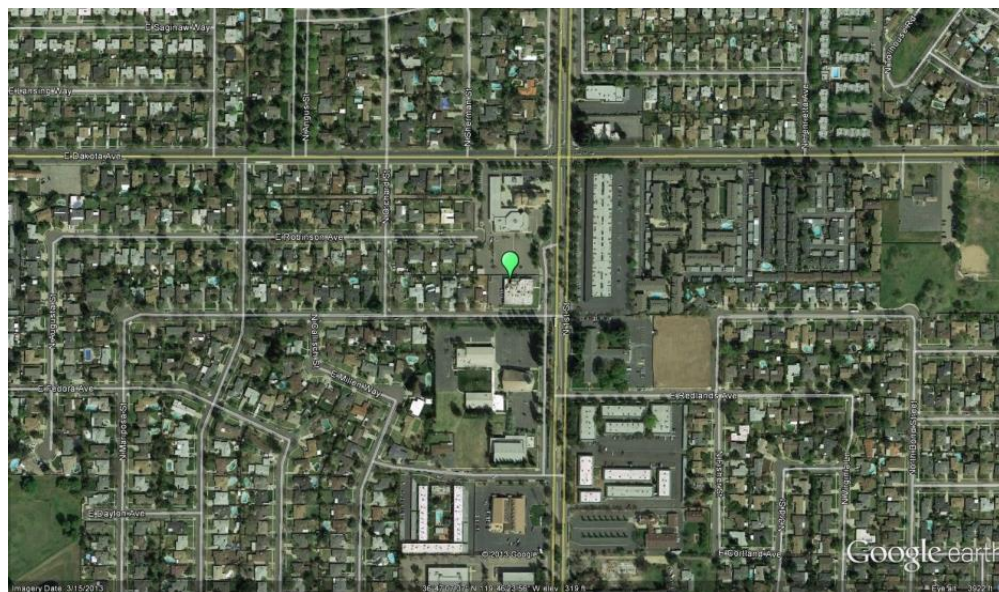


**Fresno-Pacific**

The Fresno-Pacific monitoring site is operated by SJVAPCD and is located in the Fresno, CA metropolitan area. It began operating in January 2000. The purpose of the site is to monitor representative PM2.5 concentrations in an urban area.

Site name:	Fresno-Pacific
AQS ID:	06-019-5025
County:	Fresno
Street Address:	1716 Winery Ave, Fresno, CA 93727
Geographic Coordinates:	36.7263 N, -119.7330 W
Distance to road (meters):	40 m (east)
Traffic Count (AADT; Year):	8,540; 2018*
Ground Cover:	Rubber roof coating
Representative Statistical Area (CBSA):	Fresno

\*Raw traffic count in a 24-hour period for nearest roads: Butler Ave/Winery Ave intersection  
 Source: Fresno COG Traffic Counts, 2007-2018 Kittelson & Associates, Inc.

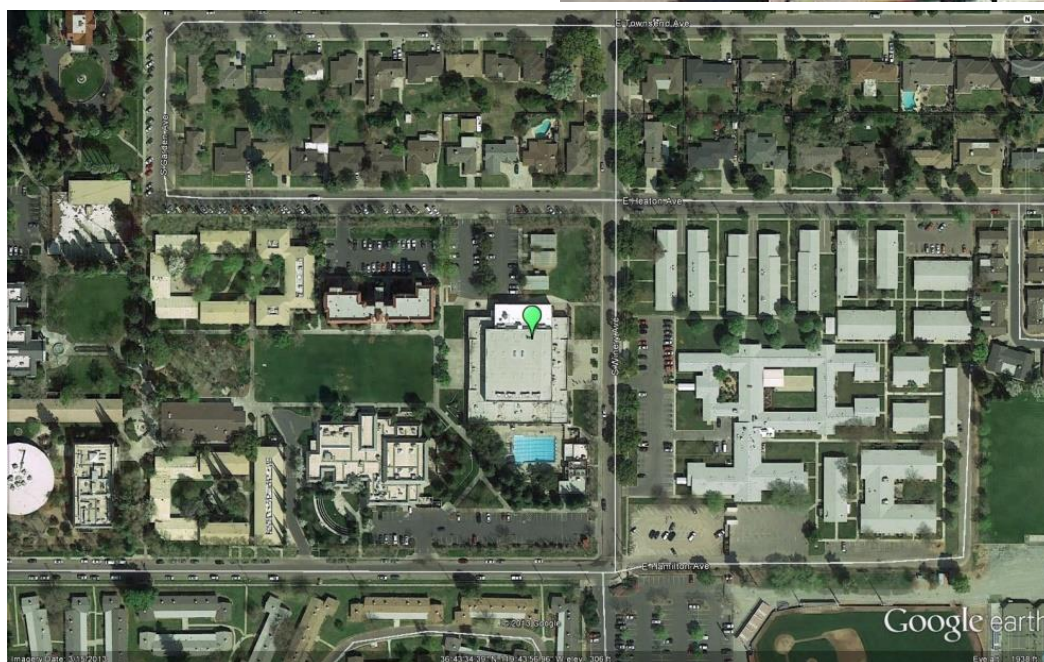


## Fresno-Foundry

The Fresno-Foundry near-road NO<sub>2</sub> monitoring site is operated by SJVAPCD and is located adjacent to Highway 99 in the Fresno, CA metropolitan area. It began operating in January 2016. The purpose of the site is to monitor representative maximum 1-hour NO<sub>2</sub> concentrations near a high traffic roadway in an urban area. In addition to NO<sub>2</sub>, the site also monitors meteorology.

Site name:	Fresno-Foundry
AQS ID:	06-019-2016
County:	Fresno
Street Address:	2482 Foundry Park Ave, Fresno, CA 93706
Geographic Coordinates:	N 36.710833, W -119.7775
Distance to road (meters):	16 to 19 meters
Traffic Count (AADT; Year):	114,000; 2016*
Ground Cover:	Paved
Representative Statistical Area (CBSA):	Fresno

\*Traffic count for nearest roads: CA Route 99 and Jensen Ave off-ramp. Source: Caltrans (2016)


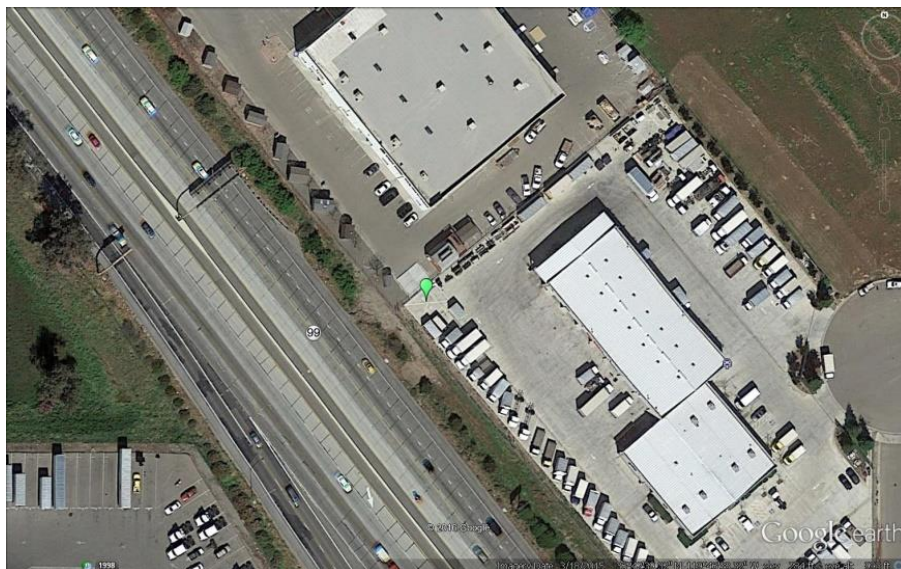


## Fresno-Drummond

The Fresno-Drummond monitoring site is operated by SJVAPCD and is located in the Fresno, CA metropolitan area. It began operating in July 1984. The purpose of the site is to monitor representative concentrations of ozone responses in an urban area. In addition to ozone, the site also monitors PM10, NO2, and meteorology.

Site name:	Fresno-Drummond
AQS ID:	06-019-0007
County:	Fresno
Street Address:	4706 E Drummond St, Fresno CA 93725
Geographic Coordinates:	36.7055 N, -119.7410 W
Distance to road (meters):	50 m (north)
Traffic Count (AADT; Year):	27,251; 2018*
Ground Cover:	Paved
Representative Statistical Area (CBSA):	Fresno

\*Raw traffic count in a 24-hour period for nearest roads: Jensen Ave between Chestnut Ave and Maple Ave  
Source: Fresno COG Traffic Counts, 2007-2018 Kittelson & Associates, Inc.

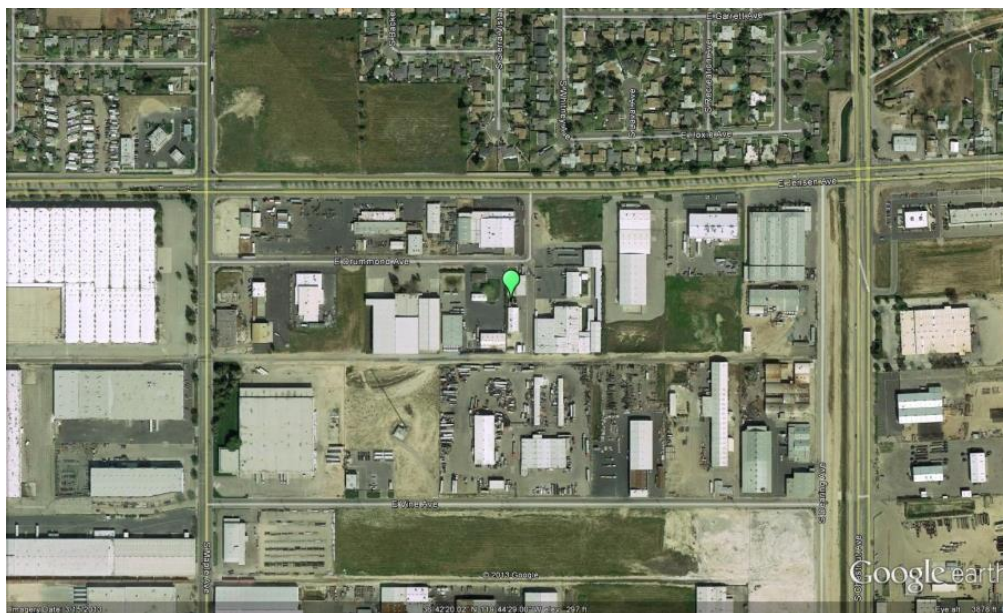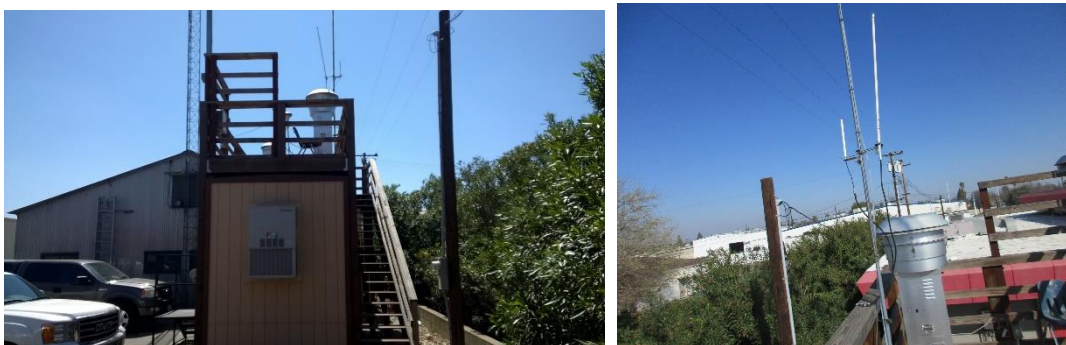


**Parlier**

The Parlier monitoring site is operated by SJVAPCD and is located 20 miles southeast of the Fresno, CA metropolitan area. It began operating in June 1983. The purpose of the site, as a PAMS Type 3 site, is to monitor maximum ozone concentrations and ozone responses from upwind urban areas. The site also monitors NO<sub>2</sub>, NMH, speciated-VOC, and meteorology for the PAMS program.

Site name:	Parlier
AQS ID:	06-019-4001
County:	Fresno
Street Address:	9240 S Riverbend Ave, Parlier CA 93648
Geographic Coordinates:	36.5972 N, -119.5040 W
Distance to road (meters):	100 m (east)
Traffic Count (AADT; Year):	21,260; 2018*
Ground Cover:	Dirt, vegetative
Representative Statistical Area (CBSA):	Fresno

\*Raw traffic count in a 24-hour period for nearest roads: E Manning Ave between S Mendocino Ave and S Newmark Ave

Source: Fresno COG Traffic Counts, 2007-2018 Kittelson & Associates, Inc.

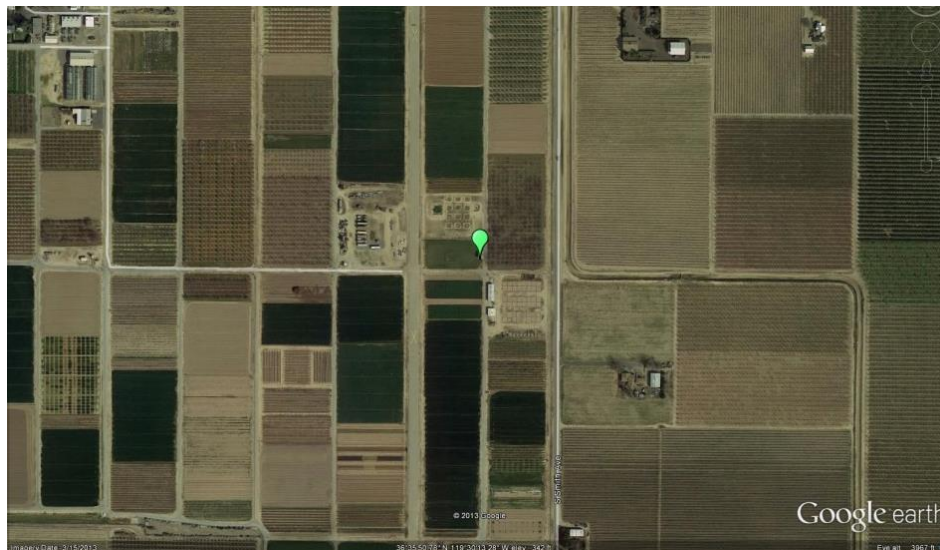

**Huron**

Huron, CA is located in southwestern Fresno County, and is about 40 miles southwest of Fresno, CA, with the coastal mountain range just to the west. North-south air flow is virtually unobstructed. This monitoring site was established in September 2009 in order to comply with Assembly Bill (AB) 841. This site monitors PM2.5 and meteorology.

Site name:	Huron
AQS ID:	06-019-2008
County:	Fresno
Street Address:	16875 4 <sup>th</sup> St, Huron, CA 93234
Geographic Coordinates:	36.2363 N, -119.7656 W
Distance to road (meters):	100 m (north)
Traffic Count (AADT; Year):	3,450; 2016*
Ground Cover:	Paved, vegetative
Representative Statistical Area (CBSA):	Fresno

\*Traffic count for nearest roads: CA Route 269 / CA Route 198. Source: Caltrans 2016




### Hanford-Irwin

The Hanford-Irwin monitoring site is operated by SJVAPCD and is located 51 miles south of the Fresno, CA metropolitan area. The site began operating in October 1993. The purpose of the site is to monitor representative concentrations of ozone, PM2.5, PM10, and NO2 responses from upwind and nearby urban areas. The site also monitors meteorology.

Site name:	Hanford-Irwin
AQS ID:	06-031-1004
County:	Kings
Street Address:	807 S Irwin St, Hanford CA 93230
Geographic Coordinates:	36.3147 N, -119.6440 W
Distance to road (meters):	60 m (east)
Traffic Count (AADT; Year):	9,647; 2016*
Ground Cover:	Paved, vegetative
Representative Statistical Area (CBSA):	Hanford – Corcoran

\*Traffic count for nearest roads: Hanford-Armona Rd east of S Williams St  
 Source: City of Hanford Public Works - Engineering, Traffic Counts Volume Summary 2017 – City of Hanford.

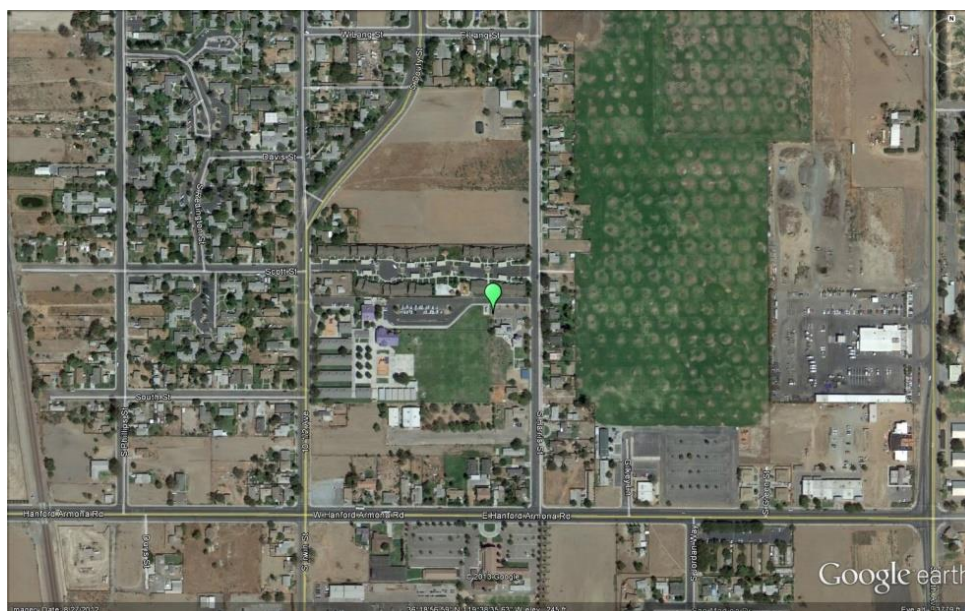




## Corcoran-Patterson

The Corcoran-Patterson monitoring site is operated by SJVAPCD and is located 67 miles south of the Fresno, CA metropolitan area. It began operating in October 1996. The site measures representative concentrations of PM10 and PM2.5. This site also monitors meteorology.

Site name:	Corcoran-Patterson
AQS ID:	06-031-0004
County:	Kings
Street Address:	1520 Patterson Ave, Corcoran CA 93212
Geographic Coordinates:	36.1022 N, -119.5660 W
Distance to road (meters):	30 m (east)
Traffic Count (AADT; Year):	3,050; 2016*
Ground Cover:	Dirt, gravel
Representative Statistical Area (CBSA):	Hanford – Corcoran

\*Traffic count for nearest roads: Junction of CA Route 43 / CA Route 137. Source: Caltrans 2016.

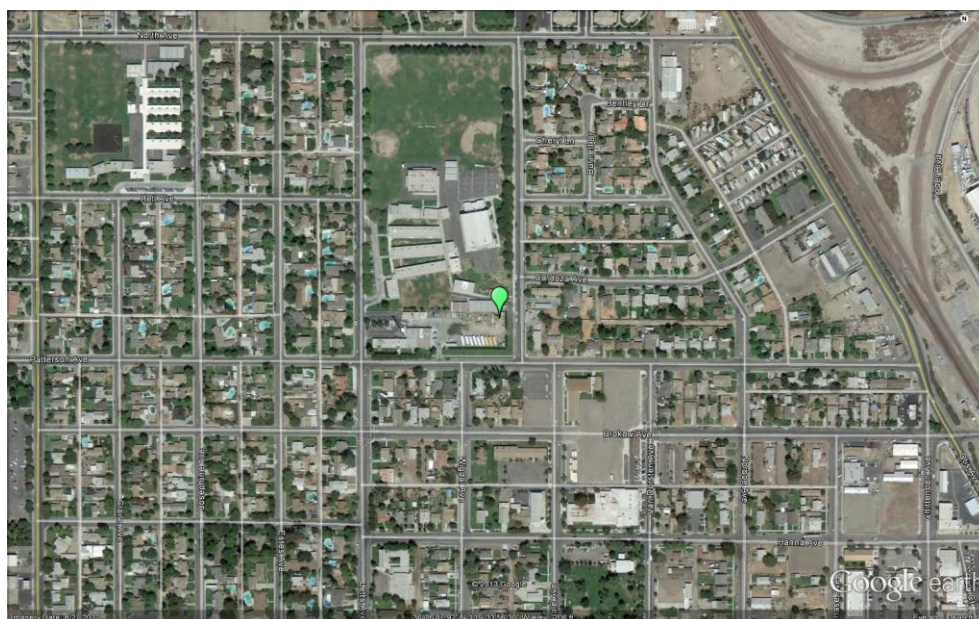


**Visalia-Airport**

The Visalia-Airport monitoring site is operated by SJVAPCD and serves as a meteorological site monitoring air temperature and relative humidity at the surface. It began reporting official meteorological data in July 1998. A lower atmosphere profiler also operates at the site measuring wind speed and wind direction.

Site name:	Visalia-Airport
AQS ID:	06-107-3000
County:	Tulare
Street Address:	9501 W Airport Dr, Visalia, CA 93277
Geographic Coordinates:	39.3266 N, -119.3984 W
Distance to road (meters):	100 m (west)
Traffic Count (AADT; Year):	65,000; 2016*
Ground Cover:	Dirt, vegetative
Representative Statistical Area (CBSA):	Visalia – Porterville

\*Traffic count for nearest roads: Junction of CA Route 99 and CA Route 198 East  
 Source: Caltrans 2016.


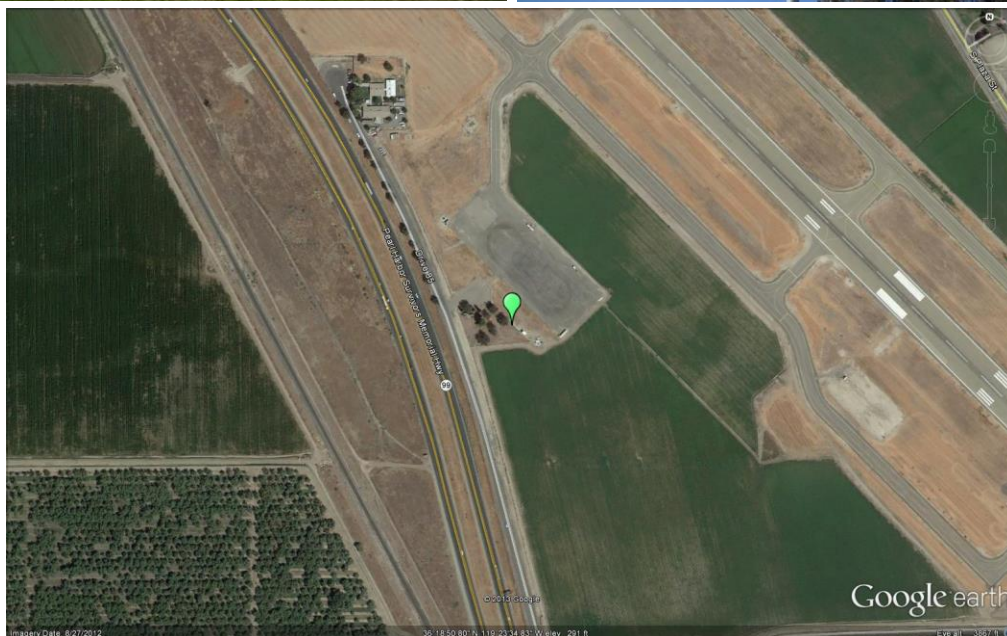


### Visalia-Church St

The Visalia-Church St monitoring site is operated by CARB. It began operating in January 1979. The purpose of the site is to monitor representative concentrations of ozone, PM2.5, and PM10 from upwind and nearby urban areas. The site also monitors NO2, PM2.5 Speciation, and meteorology.

Site name:	Visalia-Church St
AQS ID:	06-107-2002
County:	Tulare
Street Address:	310 N Church St, Visalia CA 93291
Geographic Coordinates:	36.3325 N, -119.2909 W
Distance to road (meters):	25 m (west)
Traffic Count (AADT; Year):	6,150; 2014-2015*
Ground Cover:	Paved
Representative Statistical Area (CBSA):	Visalia – Porterville

\*Traffic count for nearest roads: E Murray Ave between N Court St and N Santa Fe St  
 Source: City of Visalia Traffic and Engineering, Average Daily Traffic Volumes List 2014-2015.

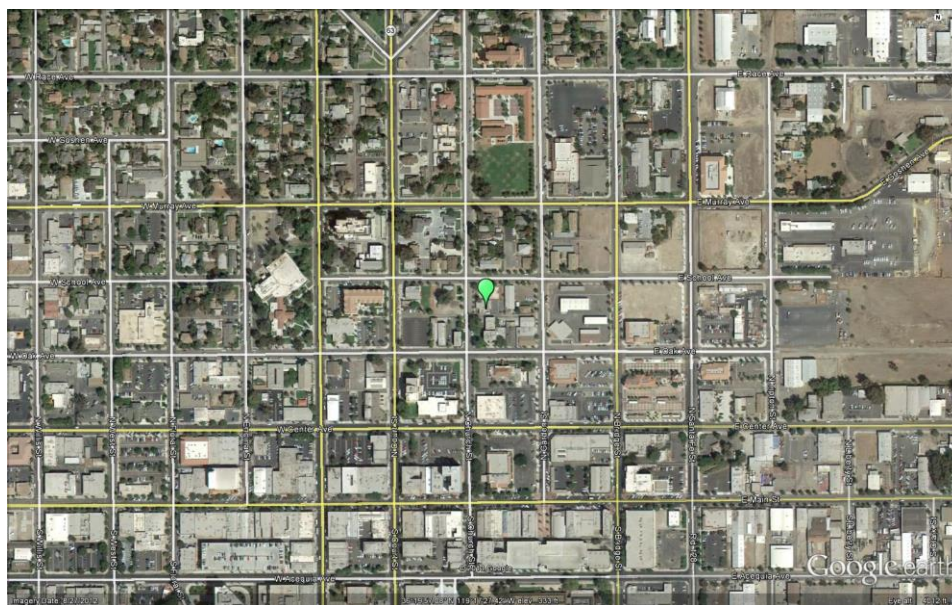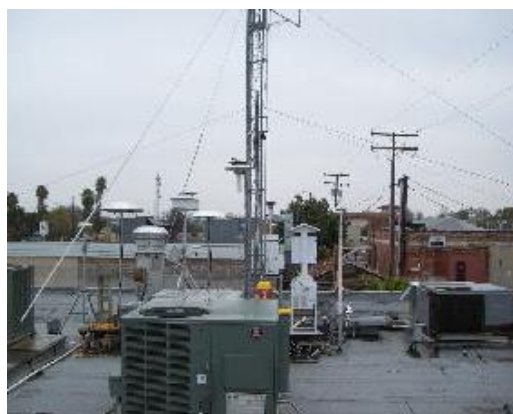


**Porterville**

The Porterville air monitoring site became operational in March 2010 and is operated by SJVAPCD. The purpose of this site is to monitor ozone, PM2.5, and meteorology.

Site name:	Porterville
AQS ID:	06-107-2010
County:	Tulare
Street Address:	1839 S Newcomb St, Porterville CA 93257
Geographic Coordinates:	36.0310 N, -119.0550 W
Distance to road (meters):	100 m (south)
Traffic Count (AADT; Year):	25,000; 2016*
Ground Cover:	Paved, vegetative
Representative Statistical Area (CBSA):	Visalia-Porterville

\*Ahead AADT traffic count for nearest roads: Junction CA Route 190/CA Route 65. Source: Caltrans 2016.

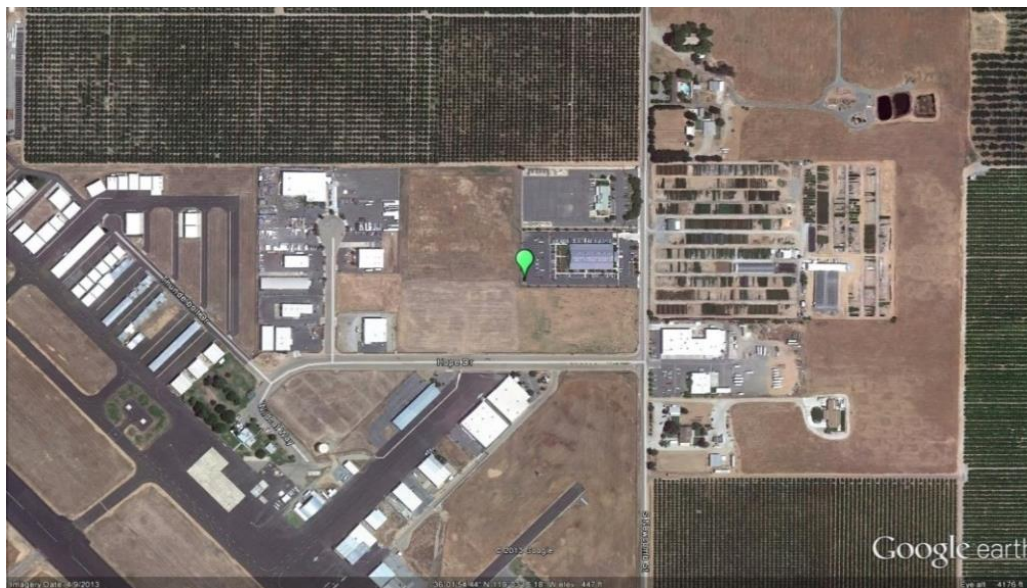


### Sequoia-Ash Mountain

The Ash Mountain monitoring station is operated by Sequoia and Kings Canyon National Park and is located at the southern entrance of the Park at 1,500-foot elevation. It began operating in July 1999, though the site has been relocated several times over the years. The site demonstrates the ozone concentrations in the foothills. The site also monitors PM2.5 and meteorology.

Site name:	Sequoia-Ash Mountain
AQS ID:	06-107-0009
County:	Tulare
Street Address:	Ash Mountain, Sequoia and Kings Canyon National Park 47050 Generals Hwy, Three Rivers, CA 93271
Geographic Coordinates:	36.4894 N, -118.8290 W
Distance to road (meters):	120 m (north)
Traffic Count (AADT; Year):	1,650: 2016*
Ground Cover:	Dirt, vegetative
Representative Statistical Area (CBSA):	Visalia – Porterville

\*CA Route 198 / Sequoia National Park boundary. Source: Caltrans Back AADT 2016

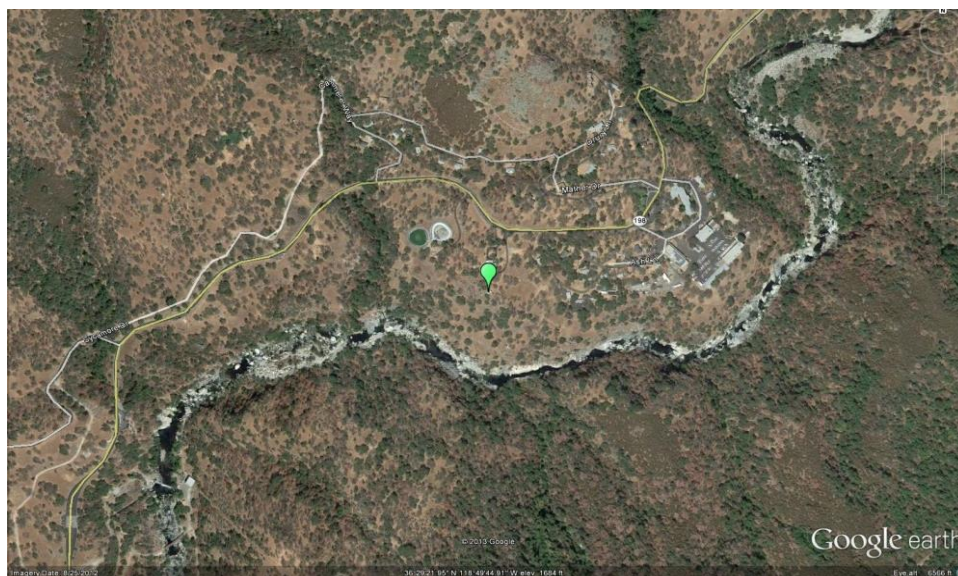


### Sequoia-Lower Kaweah

The Lower Kaweah monitoring station is operated by Sequoia and Kings Canyon National Park and is located at the southern entrance of the Park at 6,200-foot elevation. It began operating in January 1987. The site demonstrates the ozone concentrations in a rural area. The site also monitors meteorology.

Site name:	Sequoia-Lower Kaweah
AQS ID:	06-107-0006
County:	Tulare
Street Address:	Giant Forest, Sequoia National Park, 47050 Generals Highway, Three Rivers, CA 93271
Geographic Coordinates:	36.5661 N, -118.7776 W
Distance to road (meters):	380 m (southeast)
Traffic Count (AADT; Year):	1,650; 2016*
Ground Cover:	Dirt, vegetation
Representative Statistical Area (CBSA):	Visalia – Porterville

\*CA Route 198 / Sequoia National Park boundary. Source: Caltrans Back AADT 2016

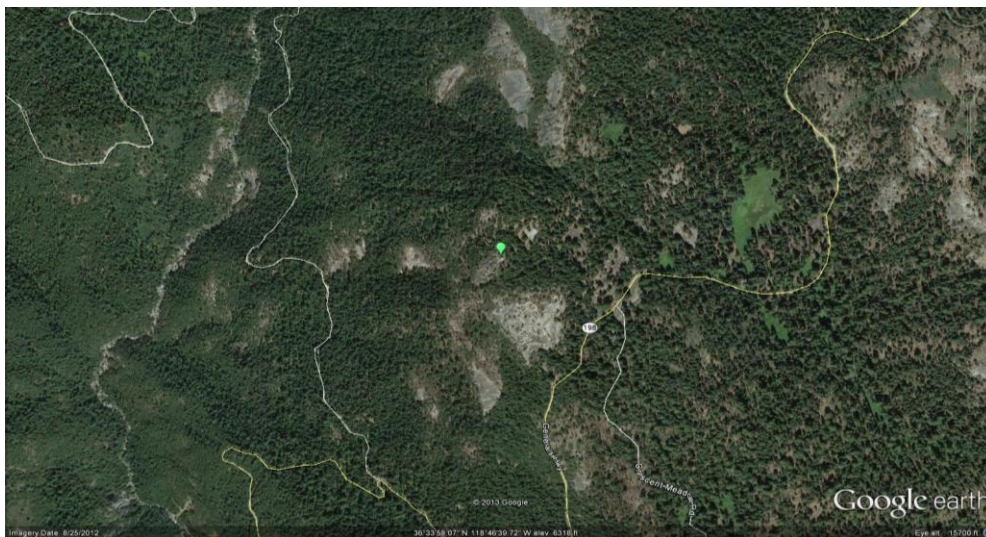


**Shafter**

The Shafter monitoring site is a shared site operated by CARB and SJVAPCD and is located 18 miles northwest of the Bakersfield, CA metropolitan area. It began operating in January 1989. This site was established as a PAMS Type 1 site, located in an area upwind of Bakersfield and not to be influenced by upwind or local ozone precursor emissions. In addition to ozone, the site also monitors NO<sub>2</sub>, NMH, speciated-VOC and meteorology for the PAMS program.

Site name:	Shafter
AQS ID:	06-029-6001
County:	Kern
Street Address:	578 Walker St, Shafter CA 93263
Geographic Coordinates:	35.5034 N, -119.2726 W
Distance to road (meters):	10 m (southwest)
Traffic Count (AADT; Year):	3,986; 2017*
Ground Cover:	Paved
Representative Statistical Area (CBSA):	Bakersfield

\*Traffic count for nearest roads: Central Ave and Walker St. Source: Kern Council of Governments.

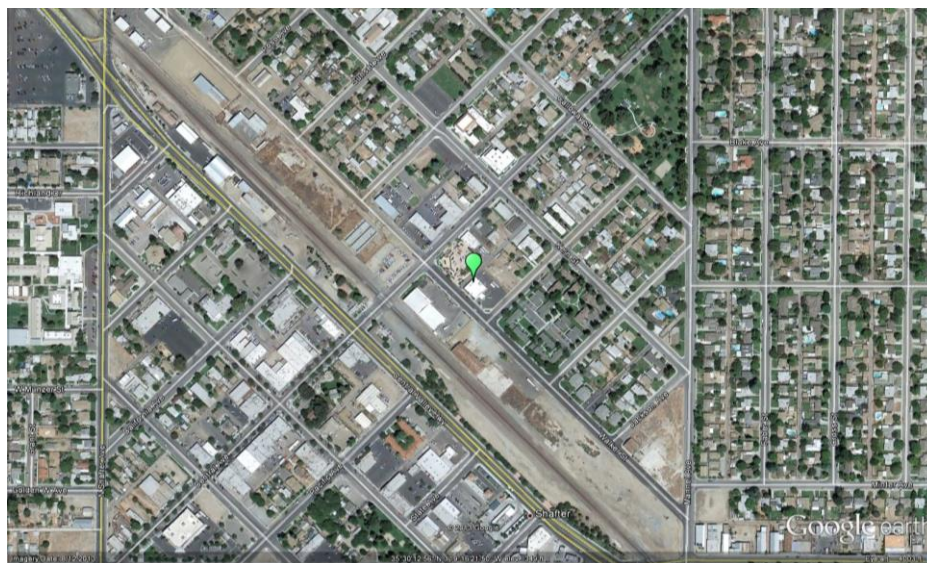


## Oildale

The Oildale monitoring site is operated by CARB and is located 6 miles north of Bakersfield, CA within the metropolitan area. It began operating in January 1980. The purpose of the site is to monitor representative concentrations of ozone and PM10. The site also monitors meteorology.

Site name:	Oildale
AQS ID:	06-029-0232
County:	Kern
Street Address:	3311 Manor St, Oildale CA 93308
Geographic Coordinates:	35.4380 N, -119.0167 W
Distance to road (meters):	150 m (northwest)
Traffic Count (AADT; Year):	7,569; 2018*
Ground Cover:	Dirt, vegetative
Representative Statistical Area (CBSA):	Bakersfield

\*Traffic count for roads: Manor St between Day Ave and Felton St. Source: Kern Council of Governments.

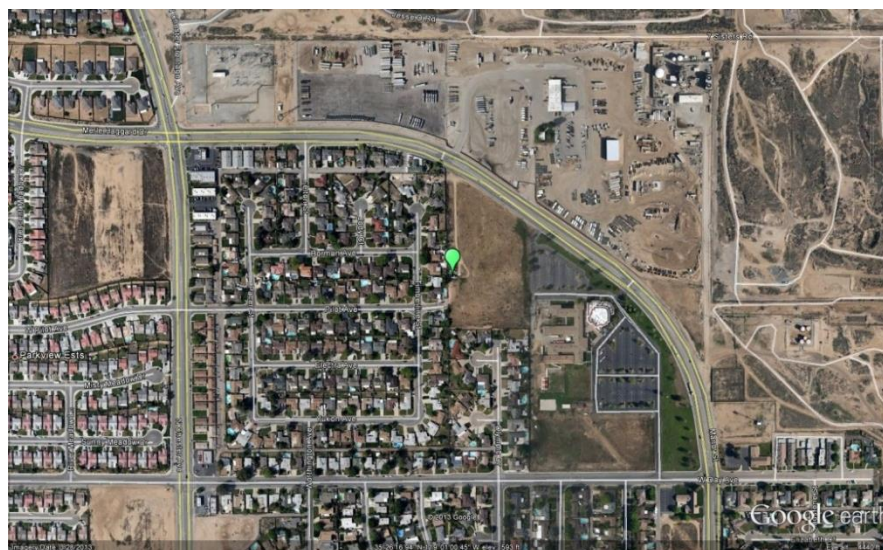



## Bakersfield-Golden / M St

The Bakersfield-Golden / M St monitoring site is operated by SJVAPCD and is located in the Bakersfield, CA metropolitan area. It began operating in June 2014. The purpose of the site is to monitor representative concentrations of PM<sub>10</sub> and PM<sub>2.5</sub> in an urban area.

Site name:	Bakersfield-Golden / M St
AQS ID:	06-029-0010
County:	Kern
Street Address:	2820 M St, Bakersfield, CA 93301
Geographic Coordinates:	35.385574 N, -119.015009 W
Distance to road (meters):	13 m
Traffic Count (AADT; Year):	4,562; 2018*
Ground Cover:	Paved
Representative Statistical Area (CBSA):	Bakersfield

\*Traffic count for nearest roads: 30th St at Golden State Ave. Source: Kern Council of Governments.




### Bakersfield-California

The Bakersfield-California monitoring site is operated by CARB and is located in the Bakersfield, CA metropolitan area. It began operating in March 1994. The purpose of the site is to monitor representative concentrations of ozone, PM10, and PM2.5 in an urban area. The Bakersfield-California site also monitors NO2, PM2.5 Speciation, Toxics, and meteorology.

Site name:	Bakersfield-California
AQS ID:	06-029-0014
County:	Kern
Street Address:	5558 California Ave, Bakersfield, CA 93309
Geographic Coordinates:	35.3566 N, -119.0626 W
Distance to road (meters):	300 m (south)
Traffic Count (AADT; Year):	33,244; 2017*
Ground Cover:	Paved
Representative Statistical Area (CBSA):	Bakersfield

\*Traffic count for roads: California Ave between Stockdale Hwy and Business Center Dr  
 Source: Kern Council of Governments

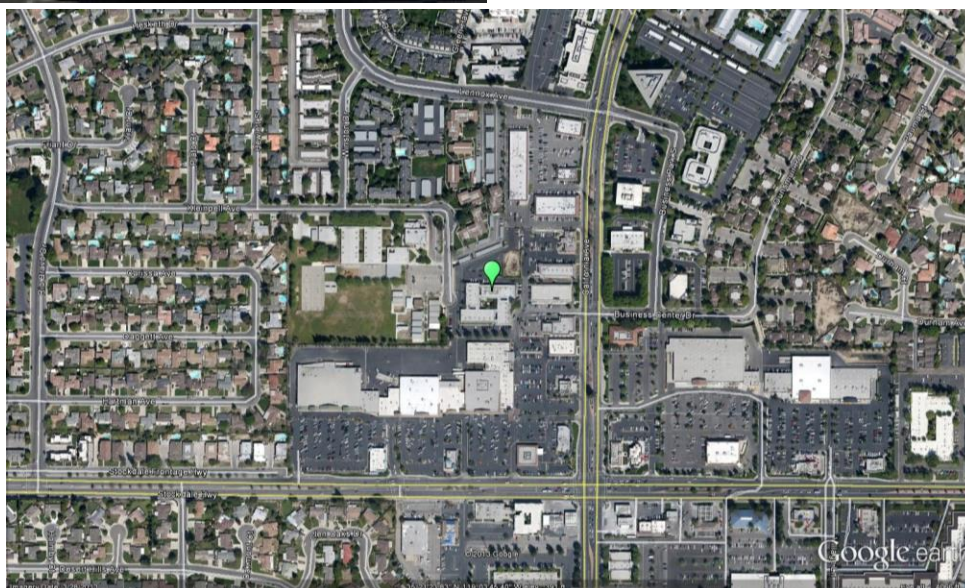

**Bakersfield-Muni**

The Bakersfield-Muni site is located in the Bakersfield, CA metropolitan area and is operated by SJVAPCD. It became operational in June 2012. The site serves as a PAMS Type 2 site and its purpose is to measure maximum ozone precursor emissions. The site monitors ozone, CO, NO2, NMH, Speciated-VOC, and meteorology for the PAMS program.

Site name:	Bakersfield-Muni
AQS ID:	06-029-2012
County:	Kern
Street Address:	2000 South Union Ave., Bakersfield, CA 93307
Geographic Coordinates:	35.3313 N, -119.0000 W
Distance to road (meters):	280 m (west)
Traffic Count (AADT; Year):	21,309; 2017* 4,594; 2017**
Ground Cover:	Paved
Representative Statistical Area (CBSA):	Bakersfield

\*Traffic count for monitoring station's street address: S Union Ave between E Casa Loma Dr and Watts Dr  
Source: Kern Council of Governments

\*\*Traffic count for road adjacent to monitoring station: Watts Dr between S Union Ave and Short St  
Source: Kern Council of Governments



### Bakersfield-Airport (Planz)


The Bakersfield-Airport (Planz) monitoring site is located in the Bakersfield, CA metropolitan area and is operated by CARB. It began operating in September 2000. The purpose of the site is to monitor representative concentrations of PM2.5 from upwind and nearby urban areas.

Site name:	Bakersfield-Airport (Planz)
AQS ID:	06-029-0016
County:	Kern
Street Address:	401 E Planz Rd, Bakersfield, CA 93307
Geographic Coordinates:	35.3246 N, -118.9976 W
Distance to road (meters):	500 m (west)
Traffic Count (AADT; Year):	17,228; 2017* 1,056; 2018**
Ground Cover:	Paved
Representative Statistical Area (CBSA):	Bakersfield

\*Traffic count for nearest cross street: S. Union Ave between E. Planz Rd and E White Lane.

Source: Kern Council of Governments

\*\*Traffic count for monitoring station's street address. Source: Kern Council of Governments

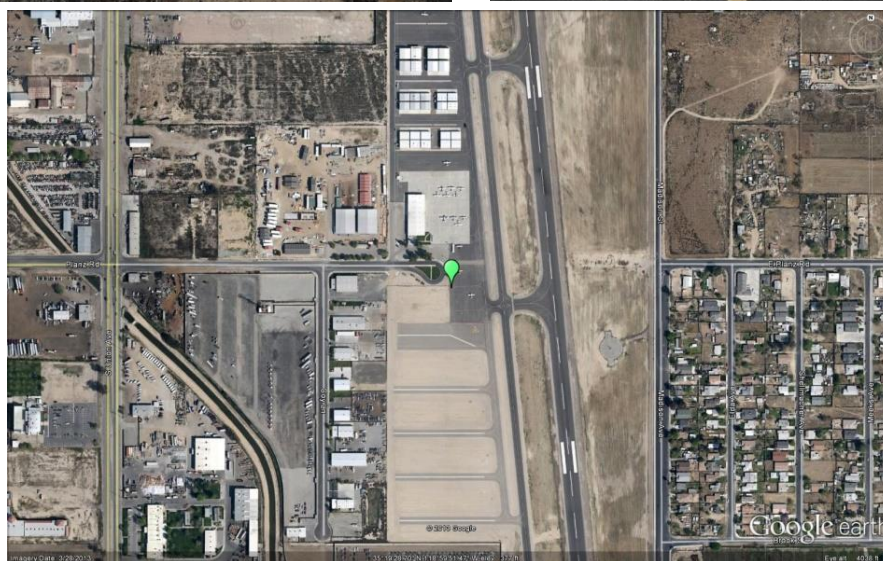


## Edison

The Edison monitoring site is operated by CARB and is located 9 miles east of the Bakersfield, CA metropolitan area. It began operating in January 1980. The purpose of the site is to monitor representative concentrations of ozone from upwind and nearby urban areas. The site also monitors NO<sub>2</sub> and meteorology.

Site name:	Edison
AQS ID:	06-029-0007
County:	Kern
Street Address:	Johnson Farm-Shed Rd, Edison CA 93320
Geographic Coordinates:	35.3456 N, -118.8518 W
Distance to road (meters):	450 m (south)
Traffic Count (AADT; Year):	2,792; 2018*
Ground Cover:	Dirt, vegetative
Representative Statistical Area (CBSA):	Bakersfield

\*Traffic count for nearest roads: Edison Hwy and Comanche Dr.  
Source: Kern Council of Governments.

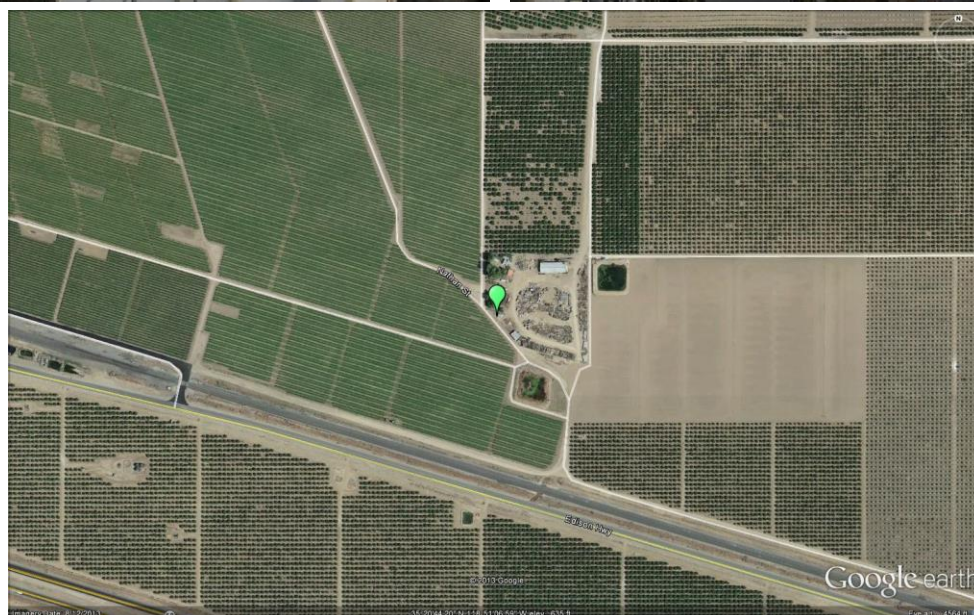

## Arvin-Di Giorgio

The Arvin-Di Giorgio site is located 18 miles southeast of the Bakersfield, CA metropolitan area. The site began operating in November 2009, and currently monitors ozone and meteorology. The purpose of this site is to measure emissions downwind of the Bakersfield urban area, and possibly serve as a PAMS Type 3 site which would monitor maximum ozone concentrations and transport from upwind urban areas. PAMS equipment at the Arvin-Di Giorgio site may be installed when space becomes available.

Site name:	Arvin-Di Giorgio
AQS ID:	06-029-5002
County:	Kern
Street Address:	19405 Buena Vista Blvd, Arvin, CA 93203
Geographic Coordinates:	35.2391 N, -118.7886 W
Distance to road (meters):	10 m (east)
Traffic Count (AADT; Year):	598; 2016*
Ground Cover:	Dirt, vegetative
Representative Statistical Area (CBSA):	Bakersfield

\*Traffic count for Buena Vista Blvd east of Tejon Hwy. Source: Kern Council of Governments.




## Maricopa

The Maricopa monitoring site is operated by SJVAPCD and is located 45 miles southwest of the Bakersfield, CA metropolitan area. It began operating in July 1987. The purpose of the site is to monitor representative concentrations of ozone in a rural area. The site also monitors meteorology.

Site name:	Maricopa
AQS ID:	06-029-0008
County:	Kern
Street Address:	755 Stanislaus St, Maricopa CA 93352
Geographic Coordinates:	35.0515 N, -119.4026 W
Distance to road (meters):	500 m (northwest)
Traffic Count (AADT; Year):	267; 2017*
Ground Cover:	Gravel, dirt, vegetative
Representative Statistical Area (CBSA):	Bakersfield

\*Traffic count for nearest roads: Union St at California St. Source: Kern Council of Governments.

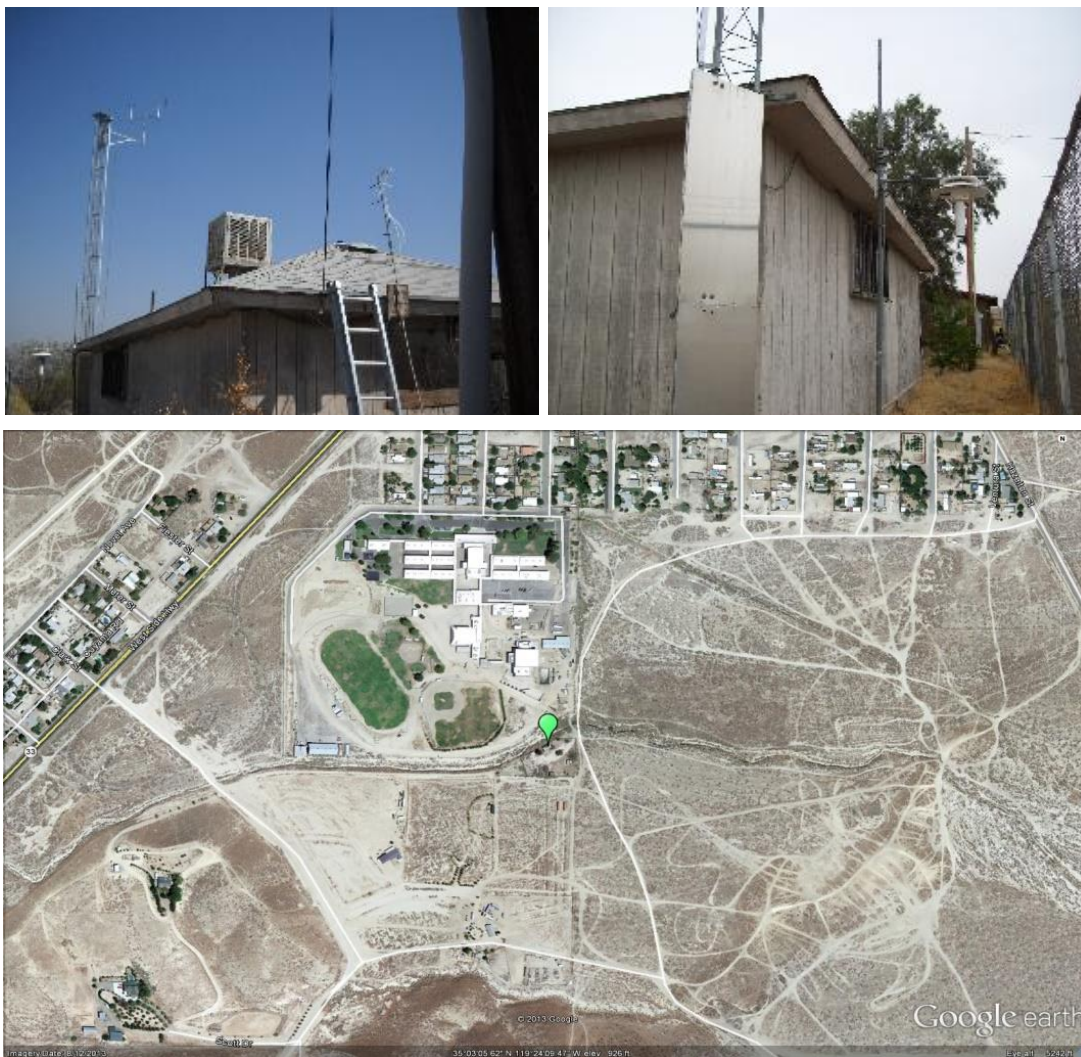


## Lebec

The Lebec monitoring station was initiated by the Tejon Ranch in 2004, and the District assumed responsibility for this site as of January 2009. This site monitors PM<sub>2.5</sub> and meteorology and allows the District to better understand pollution impacts in the southern San Emigdio Mountains. The site is also used for residential wood burning declarations for the Greater Frazier Park Area.

Site name:	Lebec
AQS ID:	06-029-2009
County:	Kern
Street Address:	1277 Beartrap Rd, Lebec, CA 93243
Geographic Coordinates:	34.8415 N, -118.8610 W
Distance to road (meters):	300 m (west)
Traffic Count (AADT; Year):	1,911; 2017*
Ground Cover:	Gravel, vegetative
Representative Statistical Area (CBSA):	Bakersfield

\*Traffic count for nearest roads: Lebec Rd and Interstate 5. Source: Kern Council of Governments.

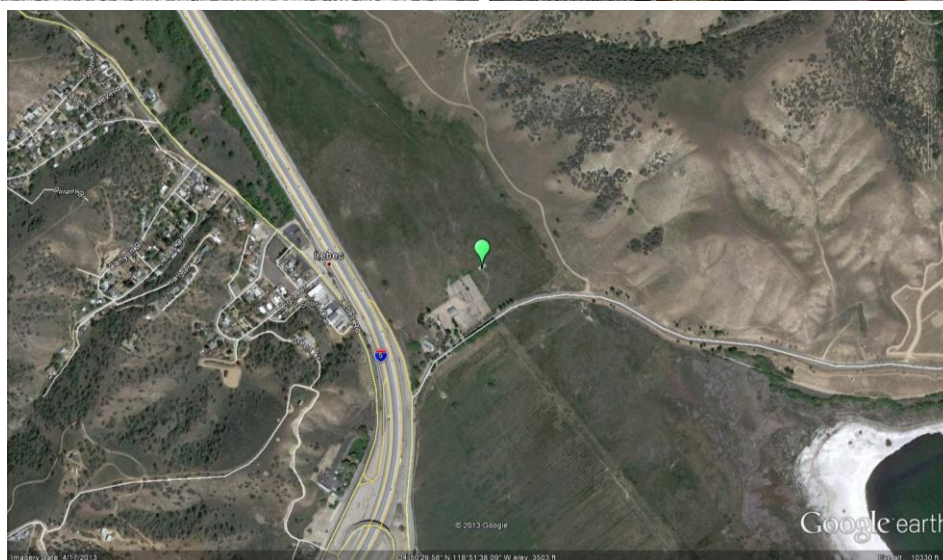



## Tribal Sites


Tribal sites are operated under the Tribal Authority Rule which is essential to tribal implementation of the CAA. Since tribal sites are not part of the District's jurisdiction, detailed site information for tribal monitors will not be provided in Appendix B.

### Picayune Rancheria

The Picayune Rancheria air monitoring site is located on tribal land in Coarsegold, Madera County, CA and is operated by the Chukchansi Indians. The site began operating in August 2011. The purpose of the site is to monitor representative concentrations of ozone, PM10, and PM2.5 on the reservation. The site also monitors meteorology.

Site name:	Picayune Rancheria
AQS ID:	06-039-0500
County:	Madera
Street Address:	46575 Road 417, Coarsegold, CA 93614
Geographic Coordinates:	37.2136 N, -119.6990 W
Distance to road (meters):	50 m (west)
Traffic Count (AADT; Year):	11,000; 2016*
Ground Cover:	Dirt, paved
Representative Statistical Area (CBSA):	Madera

\*Traffic count for CA Route 41 / Road 417. Source: Caltrans 2016 Ahead AADT


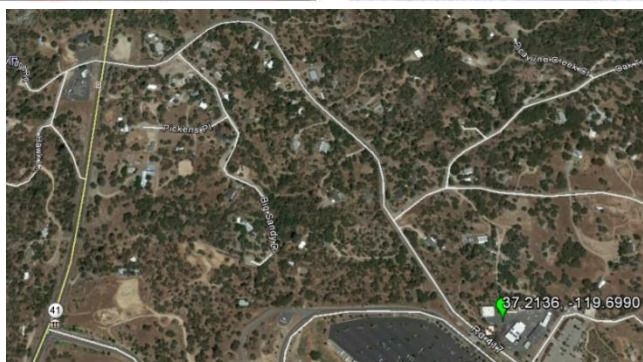


## Table Mountain Air Monitoring Site

The Table Mountain air monitoring station is located on Tribal land near Millerton Lake in Fresno County, CA and is operated by the Monache Tribe and Foothill Yokut Indians. The site began operating in September 2015. The purpose of the site is to monitor representative concentrations of ozone, PM<sub>2.5</sub>, and PM<sub>10</sub> responses from upwind and nearby urban areas. The site also monitors meteorology.

Site name:	Table Mountain Air Monitoring Site
AQS ID:	06-019-0500
County:	Fresno
Street Address:	Millerton Rd and Winchell Rd, Friant, CA 93626
Geographic Coordinates:	36.985119 N, -119.658339 W
Distance to road (meters):	Unknown
Traffic Count (AADT; Year):	47,500; 2016*
Ground Cover:	Dirt
Representative Statistical Area (CBSA):	Fresno-Madera

\*Traffic count for nearest roads: CA Route 41 and Friant Rd. Source: Caltrans 2014 Ahead AADT.

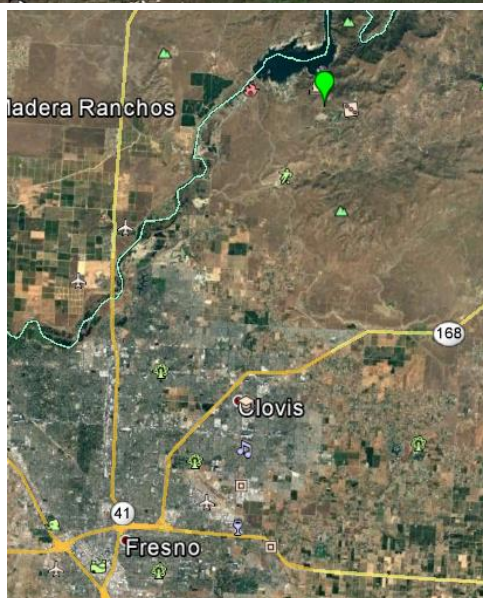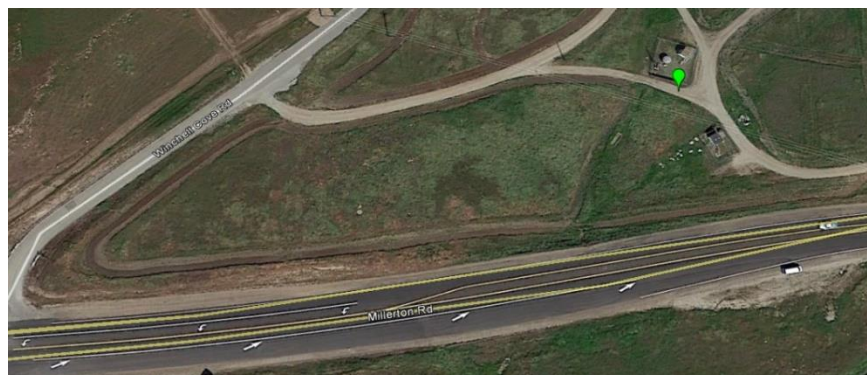



## Santa Rosa Rancheria

The Santa Rosa Rancheria air monitoring site is located on Tribal land in Lemoore, Kings County, CA and is operated by the Tachi-Yokut tribe. The site began operating in August 2006. The purpose of the site is to monitor representative concentrations of ozone and PM10 responses from upwind and nearby urban areas. The site also monitors meteorology.

Site name:	Santa Rosa Rancheria
AQS ID:	06-031-0500
County:	Kings
Street Address:	17225 Jersey Ave, Lemoore, CA 93245
Geographic Coordinates:	36.2332 N, -119.7662 W
Distance to road (meters):	40 m (south)
Traffic Count (AADT; Year):	2,430; 2006*
Ground Cover:	Dirt, paved
Representative Statistical Area (CBSA):	Hanford-Corcoran

\*Traffic count for nearest roads: 14<sup>th</sup> St between Jackson Ave and Kent Ave

Source: County of Kings 2035 General Plan – Kings County Association of Governments 2006-07 traffic data.

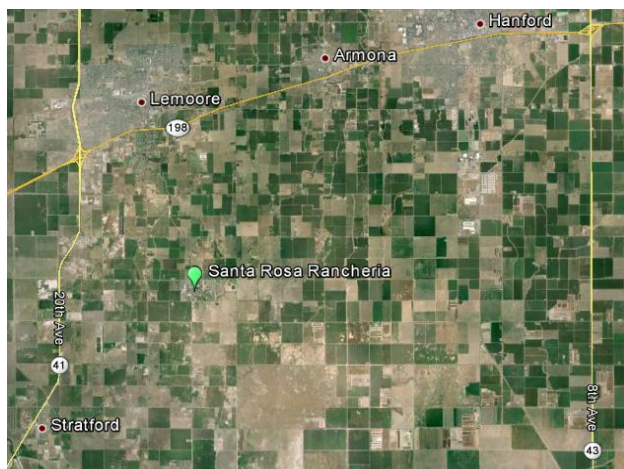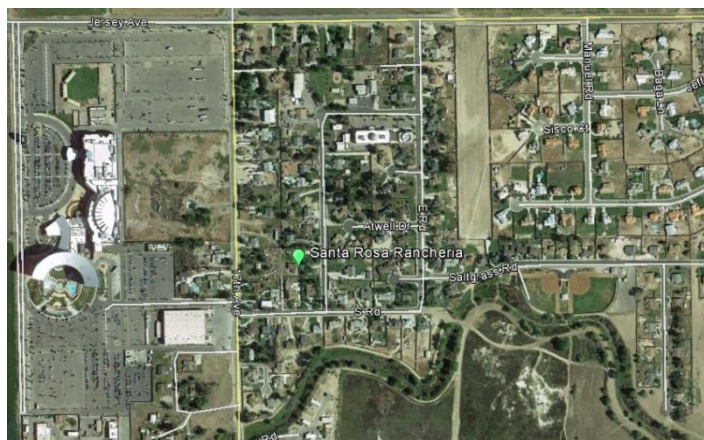

**Appendix B:  
Detailed Site Information**

This page is intentionally blank.

### List of Abbreviations

<b>Site Type</b>	
PE	Population Exposure
HC	Highest Concentration
Max PEI	Max Precursor Emissions Impact
RT	Regional Transport
GB	General/Background
SO	Source Oriented
QA	Quality Assurance Collocation
<b>Spatial Scale</b>	
N	Neighborhood
U	Urban
R	Regional
MC	Microscale
MD	Middle Scale
<b>Basic Monitoring Objective</b>	
NC	NAAQS Comparison
RS	Research
TP	Timely/Public
N/A	Not Applicable
AADT	Annual Average Daily Traffic

<b>Site Name</b>	<b>Stockton–Hazelton</b>
<b>AQS ID (XX-XXX-XXXX)</b>	06-077-1002
<b>Representative statistical area Name (i.e. MSA, CBSA, other)</b>	Stockton-Lodi
<b>County</b>	San Joaquin
<b>Collecting (Operating) Agency</b>	CARB
<b>Analytical Lab (i.e. weigh lab, toxics lab, other)</b>	CARB
<b>Reporting Agency</b>	CARB
<b>Site Start Date</b>	1/1/1976
<b>Pollutant Parameters</b>	Ozone, PM10 FRM, PM2.5 FEM, CO, NO <sub>2</sub> , Toxics
<b>Meteorological Parameters</b>	Outdoor temperature, Wind direction, Wind speed, Relative humidity
<b>Address</b>	1601 E. Hazelton St., Stockton CA 95205
<b>GPS Coordinates (decimal degrees)</b>	37.9507 N, -121.2689 W
<b>Distance to roadways</b>	62 m (north)
<b>Traffic Count/Year</b>	4000/2014 (Traffic ADT volume estimated by City of Stockton Public Works Traffic Engineering Division)
<b>Groundcover (e.g. paved, vegetative, dirt, sand, gravel)</b>	Paved

Stockton–Hazelton (1)				
Pollutant	Ozone	PM10 STP	PM2.5	PM2.5
Parameter code	44201	81102	88101	88101
Spatial scale	N	N	N	N
Site type	HC, PE	HC	HC, PE	GB, QA
Monitoring objective	NC, RS, TP	NC, RS	NC, RS, TP	TP
Monitor type	SLAMS	SLAMS	SLAMS	SLAMS *
Network affiliation	None	None	None	None
FRM/FEM/ARM/Other	FEM	FRM	FEM	FEM
POC	1	2	3	4
Primary / QA Collocated / Other (provide for all PM <sub>2.5</sub> , PM <sub>10</sub> , PM <sub>10-2.5</sub> , Pb and NO <sub>2</sub> monitors. Non-PM, Pb, NO <sub>2</sub> monitors should be listed as "N/A".)	N/A	Primary	Primary	QA Collocation
Is it suitable for comparison against the annual PM <sub>2.5</sub> ? (Y/N)	N/A	N/A	Y	Y
Instrument manufacturer and model	Teledyne API 400	Sierra Anderson 1200	Met One 1020	Met One 1020
Analysis method	UV	Gravimetric	Beta Attenuation	Beta Attenuation
Method code	087	063	170	170
Monitoring start date (MM/DD/YYYY)	01/01/1976	01/01/1985	05/11/2010	08/23/2010
Required sampling frequency (e.g. 1:3 excluding exceptional events/1:1 including exceptional events)	Hourly	1:6	Hourly	Hourly
Sampling season (MM/DD - MM/DD)	01/01 - 12/31	01/01 - 12/31	01/01 - 12/31	01/01 - 12/31
Probe/Inlet height above ground (meters)	5.7 m	6.5 m	5.7 m	5.7 m
Distance from supporting structure (meters)	2.0 m	1.7 m	2.0 m	2.0 m
Distance from obstructions on roof. Include horizontal distance + vertical height above probe for obstructions nearby. (meters)	None	None	None	None
Distance from obstructions not on roof. Include horizontal distance + vertical height above probe for obstructions nearby. (meters)	None	None	None	None

\* Per update from ARB, this QA Collocated PM<sub>2.5</sub> monitor is being reclassified as a SLAMS monitor.



Pollutant	Ozone	PM10 STP	PM2.5	PM2.5
Distance from trees (meters)	None	Airflow was obstructed by a tree near the sampler (09/2014 – 02/2017). Tree was removed in 02/2017.	None	None
Distance to furnace or incinerator flue (meters)	None	None	None	None
Distance between collocated monitors (meters)	N/A	N/A	N/A	1.2
Unrestricted airflow (degrees)	360	360	360	360
Probe material (Teflon, etc.)	Teflon	N/A	N/A	N/A
Residence time (seconds)	8.4	N/A	N/A	N/A
For low volume PM instruments (flow rate < 200 liters/minute), is any PM instrument within 1 m of the hivol? If yes, please list distance (meters) and instrument(s).	N/A	N/A	No	No
For high volume PM instrument (flow rate > 200 liters/minute), is any PM instrument within 2m of the hivol? If yes, please list distance (meters) and instrument(s).	N/A	No	N/A	N/A
Frequency of flow rate verification for manual PM samplers audit	N/A	Monthly	N/A	N/A
Frequency of flow rate verification for automated PM analyzers audit	N/A	N/A	Monthly	Monthly
Frequency of one-point QC check (gaseous)	5x/week	N/A	N/A	N/A
Last Annual Performance Evaluation (gaseous)	8/24/17	N/A	N/A	N/A
Last two semi-annual flow rate audits for PM monitors	N/A	02/13/17, 08/04/2017	02/13/17, 08/04/17	02/13/17, 08/04/17
Changes planned within the next 18 months (Y/N)	N	Y	N	N

Stockton-Hazelton (2)					
Pollutant	NO <sub>2</sub>	CO	Toxics SN20021014	Toxics SN20021016	Meteorology
Parameter code	42602	42101	Many	Many	Many
Spatial scale	N	N	N	N	R
Site type	PE	PE	PE	PE, QA	GB
Basic monitoring objective(s)	NC, RS, TP	NC, RS, TP	RS, TP	RS, TP	RS, TP
Monitor type	SLAMS	SLAMS	Many	Many	Many
Network affiliation(s), if applicable (a monitor may have none, one, or multiple)	None	None	CA Air Toxics	CA Air Toxics	None
FRM/FEM/ARM/Other	FRM	FRM	Other	Other	Other
POC	2	3	Many	Many	Many
Primary / QA Collocated / Other (provide for all PM <sub>2.5</sub> , PM <sub>10</sub> , PM <sub>10-2.5</sub> , Pb and NO <sub>2</sub> monitors. Non-PM, Pb, NO <sub>2</sub> monitors should be listed as "N/A".)	N/A	N/A	Primary	QA Collocated	Other
Is it suitable for comparison against the annual PM <sub>2.5</sub> ? (Y/N)	N/A	N/A	N/A	N/A	N/A
Instrument manufacturer and model	API 200E	API 300 EU	Xontech 924	Xontech 924	RM Young
Analysis method	CL	IR	Many	Many	Many
Method code	099	593	Many	Many	066
Monitoring start date (MM/DD/YYYY)	01/01/77	04/04/13	Varies by compound	Varies by compound	01/01/95
Required sampling frequency (e.g. 1:3 excluding exceptional events/1:1 including exceptional events)	Hourly	Hourly	Hourly	Hourly	Hourly
Sampling season (MM/DD - MM/DD)	01/01 - 12/31	01/01 - 12/31	01/01 - 12/31	01/01 - 12/31	01/01 - 12/31
Probe/Inlet height above ground (meters)	5.7 m	5.4 m	6.8 m	6.8 m	10m
Distance from supporting structure (meters)	2.0 m	N/A	2.0 m	2.0 m	None
Distance from obstructions on roof. Include horizontal distance + vertical height above probe for obstructions nearby. (meters)	N/A	N/A	N/A	N/A	N/A
Distance from obstructions not on roof. Include horizontal distance + vertical height above probe for obstructions nearby. (meters)	N/A	N/A	N/A	N/A	N/A
Distance from trees (meters)	N/A	N/A	N/A	N/A	N/A
Distance to furnace or incinerator flue (meters)	N/A	N/A	N/A	N/A	N/A

Pollutant	NO <sub>2</sub>	CO	Toxics SN20021014	Toxics SN20021016	Meteorology
Distance between collocated monitors (meters)	None	None	2.8	2.8	None
Unrestricted airflow (degrees)	360	360	360	360	360
Probe material (Teflon, etc.)	Teflon	Teflon	Teflon	Teflon	Teflon
Residence time (seconds)	8.8	6.6	N/A	N/A	N/A
For low volume PM instruments (flow rate < 200 liters/minute), is any PM instrument within 1 m of the hivol? If yes, please list distance (meters) and instrument(s).	N/A	N/A	N/A	N/A	N/A
For high volume PM instrument (flow rate > 200 liters/minute), is any PM instrument within 2m of the hivol? If yes, please list distance (meters) and instrument(s).	N/A	N/A	N/A	N/A	N/A
Frequency of flow rate verification for manual PM samplers audit	N/A	N/A	N/A	N/A	N/A
Frequency of flow rate verification for automated PM analyzers audit	N/A	N/A	N/A	N/A	N/A
Frequency of one-point QC check (gaseous)	5x/week	5x/week	N/A	N/A	N/A
Last Annual Performance Evaluation (gaseous)	8/24/17	12/6/17	8/24/17	8/24/17	N/A
Last two semi-annual flow rate audits for PM monitors	N/A	N/A	N/A	N/A	N/A
Changes planned within the next 18 months (Y/N)	N	N	N	N	N

<b>Site Name</b>	<b>Tracy - Airport</b>
<b>AQS ID (XX-XXX-XXXX)</b>	06-077-3005
<b>Representative statistical area Name (i.e. MSA, CBSA, other)</b>	Stockton-Lodi
<b>County</b>	San Joaquin
<b>Collecting (Operating) Agency</b>	SJVAPCD
<b>Analytical Lab (i.e. weigh lab, toxics lab, other)</b>	N/A
<b>Reporting Agency</b>	SJVAPCD
<b>Site Start Date</b>	01/01/2006
<b>Pollutant Parameters</b>	Ozone, PM10 FEM, PM2.5 Non-FEM, NO2
<b>Meteorological Parameters</b>	Wind speed, wind direction, outdoor temperature, barometric pressure
<b>Address</b>	5749 S. Tracy Blvd., Tracy, CA 95376
<b>GPS Coordinates (decimal degrees)</b>	37.6826 N, -121.4423 W
<b>Distance to roadways (meters)</b>	700m (east)
<b>Traffic Count/Year</b>	4,063/2014 (Traffic count for nearest roads: Linne Rd, Corral Hollow Rd) Source: TJKM Transportation Consultants
<b>Groundcover (e.g. paved, vegetative, dirt, sand, gravel)</b>	Dirt and Gravel

Tracy – Airport (1)					
Pollutant	Ozone	PM2.5	PM10	NO <sub>2</sub>	Meteorology
Parameter code	44201	88502	81102	42602	Many
Spatial scale	R	R	R	R	R
Site type	RT	RT	RT	RT	GB
Basic monitoring objective(s)	NC, RS, TP	TP	NC, RS, TP	NC, RS, TP	RS, TP
Monitor type	SLAMS	SPM	SLAMS	SLAMS	Other
FRM/FEM/ARM/Other	FEM	Non-FEM	FEM	FEM	Other
POC	1	3	3	1	Many
Primary / QA Collocated / Other (provide for all PM <sub>2.5</sub> , PM <sub>10</sub> , PM <sub>10-2.5</sub> , Pb and NO <sub>2</sub> monitors. Non-PM, Pb, NO <sub>2</sub> monitors should be listed as "N/A".)	Primary	Primary	Primary	Other	Other
Is it suitable for comparison against the annual PM <sub>2.5</sub> ? (Y/N)	N/A	N	N/A	N/A	N/A
Instrument manufacturer and model	Teledyne T400	MET One BAM 1020	Thermo TEOM 1400	Teledyne 200E	ITP- Hy-Cal 512AA3B, OT- Met One 060A-2, BP- Met One 092, WD- Met One 020C, WS-Met One 010C
Analysis method	UV	Beta-Attenuation	Tapered Element	CL	Many
Method code	087	731	079	099	Many
Monitoring start date (MM/DD/YYYY)	01/01/2006	09/27/2006	09/27/2006	01/01/2006	01/01/2006
Required sampling frequency (e.g. 1:3 excluding exceptional events/1:1 including exceptional events)	Hourly	Hourly	Hourly	Hourly	Hourly
Sampling season (MM/DD - MM/DD)	01/01 – 12/31	01/01 – 12/31	01/01 – 12/31	01/01 – 12/31	01/01 – 12/31
Probe height (meters)	5.2 m	5.6 m	5.5 m	5.2 m	10 m
Distance from supporting structure (meters)	1.9 m	1.8 m	1.7 m	1.9 m	N/A
Distance from obstructions on roof. Include horizontal distance + vertical height above probe for obstructions nearby. (meters)	N/A	N/A	N/A	N/A	N/A
Distance from obstructions not on roof. Include horizontal distance + vertical height above probe for obstructions nearby. (meters)	N/A	N/A	N/A	N/A	N/A
Distance from trees (meters)	N/A	N/A	N/A	N/A	N/A
Distance to furnace or incinerator flue (meters)	N/A	N/A	N/A	N/A	N/A

Pollutant	Ozone	PM2.5	PM10	NO <sub>2</sub>	Meteorology
Distance between monitors fulfilling a QA collocation requirement (meters).	N/A	N/A	N/A	N/A	N/A
Unrestricted airflow (degrees around probe/inlet or percentage of monitoring path)	360	360	360	360	360
Probe material for reactive gases NO/NO <sub>2</sub> /NO <sub>y</sub> , SO <sub>2</sub> , O <sub>3</sub> ; PAMS: VOCs, Carbonyls (e.g. Pyrex, stainless steel, Teflon)	Teflon/Pyrex with Borosilicate	N/A	N/A	Teflon/Pyrex with Borosilicate	N/A
Residence time for reactive gases NO/NO <sub>2</sub> /NO <sub>y</sub> , SO <sub>2</sub> , O <sub>3</sub> ; PAMS: VOCs, Carbonyls (seconds)	11.43	N/A	N/A	12.28	N/A
Frequency of one-point QC check for gaseous instruments	Daily	N/A	N/A	Daily	N/A
Frequency of flow rate verification for manual PM samplers, including Pb samplers (routine checks)	N/A	N/A	N/A	N/A	N/A
Frequency of flow rate verification for automated PM analyzers (routine checks)	N/A	Bi-Weekly	Monthly	N/A	N/A
For low volume PM instruments (flow rate < 200 liters/minute), is any PM instrument within 1 m of the hivol? If yes, please list distance (meters) and instrument(s).	N/A	No	No	N/A	N/A
For high volume PM instrument (flow rate > 200 liters/minute), is any PM instrument within 2m of the hivol? If yes, please list distance (meters) and instrument(s).	N/A	N/A	N/A	N/A	N/A
Date of Annual Performance Evaluation conducted in the past calendar year for gaseous parameters (MM/DD/YYYY)	11/16/17	N/A	N/A	11/16/17	N/A
Date of two semi-annual flow rate audits conducted in the past calendar year for PM monitors (MM/DD/YYYY, MM/DD/YYYY)	N/A	05/03/17, 11/16/17	05/03/17, 11/16/17	N/A	N/A
Changes planned within the next 18 months (Y/N)	N	N	N	N	Yes, potential closure of lower air profiler due to changes to PAMS program requirements.

<b>Site Name</b>	<b>Manteca</b>
<b>AQS ID (XX-XXX-XXXX)</b>	06-077-2010
<b>Representative statistical area Name (i.e. MSA, CBSA, other)</b>	Stockton-Lodi
<b>County</b>	San Joaquin
<b>Collecting (Operating) Agency</b>	SJVAPCD
<b>Analytical Lab (i.e. weigh lab, toxics lab, other)</b>	N/A
<b>Reporting Agency</b>	SJVAPCD
<b>Site Start Date</b>	11/16/2010
<b>Pollutant Parameters</b>	PM2.5 FEM; PM10 FEM
<b>Meteorological Parameters</b>	Wind speed, wind direction, outdoor temperature, barometric pressure
<b>Address</b>	530 Fishback Rd., Manteca, CA 95337
<b>GPS Coordinates (decimal degrees)</b>	37.7933 N, -121.2477 W
<b>Distance to roadways (meters)</b>	12 m (west)
<b>Traffic Count/Year</b>	13,383 / 2014 (Traffic count for nearest roads: Yosemite Ave and Airport Way) Source: TJKM Transportation Consultants
<b>Groundcover (e.g. paved, vegetative, dirt, sand, gravel)</b>	Paved, vegetative

Manteca (1)						
Pollutant	PM2.5	PM10	PM2.5	PM10 LC	PM10 STP	Meteorology
Parameter code	88101	81102	88101	85101	81102	
Spatial scale	N	N	N	N	N	N
Site type	PE	PE	HC	HC	HC	PE
Basic monitoring objective(s)	NC, RS, TP	NC, RS, TP	NC, RS, TP	RS, TP	NC, RS, TP	RS, TP
Monitor type	SLAMS	SLAMS	SLAMS	SLAMS	SLAMS	Other
Network affiliation(s), if applicable (a monitor may have none, one, or multiple)	None	None	None	None	None	None
FRM/FEM/ARM/Other	FEM	FEM	FEM	FEM	FEM	Other
POC	3	3	3	3	3	1
Primary / QA Collocated / Other (provide for all PM <sub>2.5</sub> , PM <sub>10</sub> , PM <sub>10-2.5</sub> , Pb and NO <sub>2</sub> monitors. Non-PM, Pb, NO <sub>2</sub> monitors should be listed as "N/A".)	Primary	Primary	QA Collocated	Other	Primary	Other
Is it suitable for comparison against the annual PM <sub>2.5</sub> ? (Y/N)	Yes	N/A	Yes	N/A	N/A	N/A
Instrument manufacturer and model	MET One BAM 1020	Thermo TEOM 1400	Teledyne 602	Teledyne 602	Teledyne 602	ITP – Hy-Cal 512AA3B, OT – Met One 060A-2, BP – Met One 092, WD – Met One 020C, WS – Met One 010C
Analysis method	Beta Attenuation	Gravimetric	Beta Attenuation	Beta Attenuation	Beta Attenuation	Many
Method code	170	079	205	204	204	Many
Monitoring start date (MM/DD/YYYY)	11/16/2010	05/02/2011	01/01/2017	01/01/2017	01/01/2017	11/16/2010
Required sampling frequency (e.g. 1:3 excluding exceptional events/1:1 including exceptional events)	Hourly	Hourly	Hourly	Hourly	Hourly	Hourly
Sampling season (MM/DD - MM/DD)	01/01 – 12/31	01/01 – 12/31	01/01 - 12/31	01/01 - 12/31	01/01 - 12/31	01/01 – 12/31



<b>Pollutant</b>	<b>PM2.5</b>	<b>PM10</b>	<b>PM2.5</b>	<b>PM10 LC</b>	<b>PM10 STP</b>	<b>Meteorology</b>
Probe height (meters)	4.8 m	5 m	4 m	4.1 m	4.1 m	10 m
Distance from supporting structure (meters)	1.73 m	1.95 m	1.2 m	2 m	2 m	0 m
Distance from obstructions on roof. Include horizontal distance + vertical height above probe for obstructions nearby. (meters)	N/A	N/A	N/A	N/A	N/A	N/A
Distance from obstructions not on roof. Include horizontal distance + vertical height above probe for obstructions nearby. (meters)	N/A	N/A	N/A	N/A	N/A	N/A
Distance from trees (meters)	55 m	55 m	55 m	55 m	55 m	55.5 m
Distance to furnace or incinerator flue (meters)	N/A	N/A	N/A	N/A	N/A	N/A
Distance between monitors fulfilling a QA collocation requirement (meters).	N/A	N/A	N/A	N/A	N/A	N/A
Unrestricted airflow (degrees around probe/inlet or percentage of monitoring path)	360	360	360	360	360	360
Probe material for reactive gases NO/NO <sub>2</sub> /NO <sub>y</sub> , SO <sub>2</sub> , O <sub>3</sub> ; PAMS: VOCs, Carbonyls (e.g. Pyrex, stainless steel, Teflon)	N/A	N/A	N/A	N/A	N/A	N/A
Residence time for reactive gases NO/NO <sub>2</sub> /NO <sub>y</sub> , SO <sub>2</sub> , O <sub>3</sub> ; PAMS: VOCs, Carbonyls (seconds)	N/A	N/A	N/A	N/A	N/A	N/A
Frequency of one-point QC check for gaseous instruments	N/A	N/A	N/A	N/A	N/A	N/A
Frequency of flow rate verification for manual PM samplers, including Pb samplers (routine checks)	N/A	N/A	N/A	N/A	N/A	N/A

Pollutant	PM2.5	PM10	PM2.5	PM10 LC	PM10 STP	Meteorology
Frequency of flow rate verification for automated PM analyzers (routine checks)	Biweekly	Biweekly	Biweekly	Biweekly	Biweekly	N/A
For low volume PM instruments (flow rate < 200 liters/minute), is any PM instrument within 1 m of the hivol? If yes, please list distance (meters) and instrument(s).	No	No	No	No	No	N/A
For high volume PM instrument (flow rate > 200 liters/minute), is any PM instrument within 2m of the hivol? If yes, please list distance (meters) and instrument(s).	N/A	N/A	N/A	N/A	N/A	N/A
Date of Annual Performance Evaluation conducted in the past calendar year for gaseous parameters (MM/DD/YYYY)	N/A	N/A	N/A	N/A	N/A	N/A
Date of two semi-annual flow rate audits conducted in the past calendar year for PM monitors (MM/DD/YYYY, MM/DD/YYYY)	05/03/17, 11/13/17	05/03/17, 11/13/17	None yet	None yet	None yet	N/A
Changes planned within the next 18 months (Y/N)	Removed 12/12/2017	Removed 12/12/2017	Started sampling 12/12/2017	Started sampling 12/12/2017	Started sampling 12/12/2017	N

<b>Site Name</b>	<b>Modesto –14<sup>th</sup> St</b>
<b>AQS ID (XX-XXX-XXXX)</b>	06-099-0005
<b>Representative statistical area Name (i.e. MSA, CBSA, other)</b>	Modesto
<b>County</b>	Stanislaus
<b>Collecting (Operating) Agency</b>	CARB
<b>Analytical Lab (i.e. weigh lab, toxics lab, other)</b>	CARB
<b>Reporting Agency</b>	CARB
<b>Site Start Date</b>	01/01/81
<b>Pollutant Parameters</b>	Ozone, PM10 FEM, PM2.5 FRM, PM2.5 FEM, CO, PM2.5 Speciation
<b>Meteorological Parameters</b>	Wind speed, wind direction, outdoor temperature, relative humidity
<b>Address</b>	814 14th Street, Modesto CA 95354
<b>GPS Coordinates (decimal degrees)</b>	37.6421 N, -120.9942 W
<b>Distance to road</b>	50 m (southwest)
<b>Traffic Count/Year</b>	122,000/2014 (Traffic count for nearest roads: H Street / Rte 99, Source: Caltrans 2016 AADDT)
<b>Groundcover (e.g. paved, vegetative, dirt, sand, gravel)</b>	Paved

<b>Modesto –14<sup>th</sup> St (1)</b>			
<b>Pollutant</b>	<b>Ozone</b>	<b>PM10 STP</b>	<b>PM2.5</b>
Parameter code	44201	81102	88101
Spatial scale	N	N	N
Site type	HC, PE	PE	PE
Monitoring objective	NC, RS, TP	NC, RS, TP	NC, RS, TP
Monitor type	SLAMS	SLAMS	SLAMS
Network affiliation	None	None	None
FRM/FEM/ARM/Other	FEM	FEM	FEM
POC	1	7	3
Primary / QA Collocated / Other (provide for all PM <sub>2.5</sub> , PM <sub>10</sub> , PM <sub>10-2.5</sub> , Pb and NO <sub>2</sub> monitors. Non-PM, Pb, NO <sub>2</sub> monitors should be listed as "N/A".)	N/A	Primary	Primary
Is it suitable for comparison against the annual PM <sub>2.5</sub> ? (Y/N)	N/A	N/A	Y
Instrument manufacturer and model	Teledyne API 400	Met One 4 Models Beta A	Met One 1020
Analysis method	UV	Beta Attenuation	Beta Attenuation
Method code	087	122	170
Monitoring start date (MM/DD/YYYY)	1/1/1981	12/1/2013	5/1/2010
Required sampling frequency (e.g. 1:3 excluding exceptional events/1:1 including exceptional events)	Hourly	Hourly	Hourly
Sampling season (MM/DD - MM/DD)	01/01 - 12/31	01/01 - 12/31	01/01 - 12/31
Probe/Inlet height above ground (meters)	7.9 m	4.4 m	5.1 m
Distance from supporting structure (meters)	4.8 m	1.1 m	1.8 m
Distance from obstructions on roof. Include horizontal distance + vertical height above probe for obstructions nearby. (meters)	N/A	N/A	N/A
Distance from obstructions not on roof. Include horizontal distance + vertical height above probe for obstructions nearby. (meters)	N/A	N/A	N/A
Distance from trees (meters)	N/A	N/A	N/A
Distance to furnace or incinerator flue (meters)	N/A	N/A	N/A
Distance between collocated monitors (meters)	N/A	N/A	2.0
Unrestricted airflow (degrees)	360	360	360
Probe material (Teflon, etc.)	Teflon	N/A	N/A
Residence time (seconds)	9.3	N/A	N/A

Pollutant	Ozone	PM10 STP	PM2.5
For low volume PM instruments (flow rate < 200 liters/minute), is any PM instrument within 1 m of the hivol? If yes, please list distance (meters) and instrument(s).	N/A	No	No
For high volume PM instrument (flow rate > 200 liters/minute), is any PM instrument within 2m of the hivol? If yes, please list distance (meters) and instrument(s).	N/A	N/A	N/A
Frequency of flow rate verification for manual PM samplers audit	N/A	N/A	N/A
Frequency of flow rate verification for automated PM analyzers audit	N/A	Monthly	Bi-Weekly
Frequency of one-point QC check (gaseous)	5x/week	N/A	N/A
Last Annual Performance Evaluation (gaseous)	11/29/17	N/A	N/A
Last two semi-annual flow rate audits for PM monitors	N/A	5/05/2017, 11/29/2017	5/05/2017, 11/29/2017
Changes planned within the next 18 months (Y/N)	N	N	N

Modesto-14 <sup>th</sup> St (2)				
Pollutant	PM2.5	PM2.5 Speciation	CO	Meteorology
Parameter code	88101	Many	42101	Many
Spatial scale	N	N	N	R
Site type	PE, QA	PE	PE	GB
Monitoring objective(s)	NC, RS	RS	NC, RS, TP	RS, TP
Monitor type	SLAMS	SLAMS	SLAMS	SLAMS
Network affiliation	None	CSN Supplemental	None	None
FRM/FEM/ARM/Other	FRM	Other	FRM	Other
POC	1	5	3	Many
Primary / QA Collocated / Other (provide for all PM <sub>2.5</sub> , PM <sub>10</sub> , PM <sub>10-2.5</sub> , Pb and NO <sub>2</sub> monitors. Non-PM, Pb, NO <sub>2</sub> monitors should be listed as "N/A".)	QA Collocation	Primary	N/A	Other
Is it suitable for comparison against the annual PM <sub>2.5</sub> ? (Y/N)	Y	N/A	N/A	N/A
Instrument manufacturer and model	Thermo 2000i	Met-One SASS	API 300 EU	N/A
Analysis method	Gravimetric	Many	IR	N/A
Method code	143	810	593	066

Pollutant	PM2.5	PM2.5 Speciation	CO	Meteorology
Monitoring start date (MM/DD/YYYY)	01/03/95	01/14/02	01/01/13	01/01/95
Required sampling frequency (e.g. 1:3 excluding exceptional events/1:1 including exceptional events)	1:12	1:6	Hourly	Hourly
Sampling season (MM/DD - MM/DD)	01/01 - 12/31	01/01 - 12/31	01/01 - 12/31	01/01 - 12/31
Probe/Inlet height above ground (meters)	6.1 m	5.6 m	7.7 m	N/A
Distance from supporting structure (meters)	2.8 m	N/A	1.0 m (per most recent ARB audit)	N/A
Distance from obstructions on roof. Include horizontal distance + vertical height above probe for obstructions nearby. (meters)	N/A	4.5 m	N/A	N/A
Distance from obstructions not on roof. Include horizontal distance + vertical height above probe for obstructions nearby. (meters)	N/A	1 m (Met tower)	N/A	N/A
Distance from trees (meters)	N/A	40 m	N/A	N/A
Distance to furnace or incinerator flue (meters)	N/A	Approx. 40 m	N/A	N/A
Distance between collocated monitors (meters)	2.0	2.4 m (URG 3000n) 4.5 m (Partisol) 3.0 m (BAM-10)	N/A	N/A
Unrestricted airflow (degrees)	360	Est. 350	360	360
Probe material (Teflon, etc.)	N/A	N/A	Teflon	N/A
Residence time (seconds)	N/A	N/A	9.5	N/A
For low volume PM instruments (flow rate < 200 liters/minute), is any PM instrument within 1 m of the inlet? If yes, please list distance (meters) and instrument(s).	N/A	N/A	N/A	N/A
For high volume PM instrument (flow rate > 200 liters/minute), is any PM instrument within 2m of the inlet? If yes, please list distance (meters) and instrument(s).	N/A	N/A	N/A	N/A
Frequency of flow rate verification for manual PM samplers audit	Monthly	Monthly	N/A	N/A
Frequency of flow rate verification for automated PM analyzers audit	N/A	N/A	N/A	N/A
Frequency of one-point QC check (gaseous)	N/A	N/A	5x/week	N/A

<b>Pollutant</b>	<b>PM2.5</b>	<b>PM2.5 Speciation</b>	<b>CO</b>	<b>Meteorology</b>
Last Annual Performance Evaluation (gaseous)	N/A	N/A	12/6/17	N/A
Last two semi-annual flow rate audits for PM monitors	5/05/2017, 11/29/2017	5/05/2017	N/A	N/A
Changes planned within the next 18 months (Y/N)	N	N	N	N

<b>Site Name</b>	<b>Turlock</b>	
<b>AQS ID (XX-XXX-XXXX)</b>	06-099-0006	
<b>Representative statistical area Name (i.e. MSA, CBSA, other)</b>	Modesto	
<b>County</b>	Stanislaus	
<b>Collecting (Operating) Agency</b>	SJVAPCD	
<b>Analytical Lab (i.e. weigh lab, toxics lab, other)</b>	CARB	
<b>Reporting Agency</b>	SJVAPD: Ozone, PM2.5 FEM, NO2, Meteorology	CARB: PM10 FRM
<b>Site Start Date</b>	4/1/1992	
<b>Pollutant Parameters</b>	Ozone, PM10 FRM, PM2.5 FEM, NO2	
<b>Meteorological Parameters</b>	Wind speed, wind direction, outdoor temperature, barometric pressure	
<b>Address</b>	900 S. Minaret St., Turlock, CA 95380	
<b>GPS Coordinates (decimal degrees)</b>	37.4880 N, -120.8360 W	
<b>Distance to roadways (meters)</b>	40m (northeast)	
<b>Traffic Count/Year</b>	7,186/2015 (Minaret Street/East F Street near Golden State Blvd., Source: City of Turlock Engineering Division 2015)	
<b>Groundcover (e.g. paved, vegetative, dirt, sand, gravel)</b>	Gravel	



Turlock (1)					
Pollutant	Ozone	PM2.5	PM10	NO <sub>2</sub>	Meteorology
Parameter code	44201	88101	81102	42602	Many
Spatial scale	N	N	N	N	R
Site type	HC, PE	HC, PE	PE	PE	GB
Basic monitoring objective(s)	NC, RS, TP	NC, RS, TP	NC, RS	NC, RS, TP	RS, TP
Monitor type	SLAMS	SLAMS	SLAMS	SLAMS	Other
Network affiliation(s), if applicable (a monitor may have none, one, or multiple)	None	None	None	None	None
FRM/FEM/ARM/Other	FEM	FEM	FRM	FEM	Other
POC	1	3	1	1	1
Primary / QA Collocated / Other (provide for all PM <sub>2.5</sub> , PM <sub>10</sub> , PM <sub>10-2.5</sub> , Pb and NO <sub>2</sub> monitors. Non-PM, Pb, NO <sub>2</sub> monitors should be listed as "N/A".)	N/A	Primary	Primary	N/A	Other
Is it suitable for comparison against the annual PM <sub>2.5</sub> ? (Y/N)	N/A	Y	N/A	N/A	N/A
Instrument manufacturer and model	Teledyne T400	MET One BAM 1020	ECOTECH Hi-Vol 3000	Teledyne 200E	ITP- Hy-Cal 512AA3B, OT- Met One 060A-2, BP- Met One 092, WD- Met One 020C, WS-Met One 010C
Analysis method	UV	Beta Attenuation	Gravimetric	Chem.	Many
Method code	087	170	162	099	Many
Monitoring start date (MM/DD/YYYY)	04/01/2000	09/14/2006	09/14/2006	04/01/2000	WS, WD - 4/1/2000; OT, BP 09/03/08
Required sampling frequency (e.g. 1:3 excluding exceptional events/1:1 including exceptional events)	Hourly	Hourly	1:6	Hourly	Hourly
Sampling season (MM/DD - MM/DD)	01/01 - 12/31	01/01 - 12/31	01/01 - 12/31	01/01 - 12/31	01/01 - 12/31
Probe height (meters)	5.6 m	5.6 m	5.5 m	5.6 m	8.3 m
Distance from supporting structure (meters)	2 m	2 m	2 m	2 m	N/A

Pollutant	Ozone	PM2.5	PM10	NO <sub>2</sub>	Meteorology
Distance from obstructions on roof. Include horizontal distance + vertical height above probe for obstructions nearby. (meters)	N/A	N/A	N/A	N/A	N/A
Distance from obstructions not on roof. Include horizontal distance + vertical height above probe for obstructions nearby. (meters)	N/A	N/A	N/A	N/A	N/A
Distance from trees (meters)	37.5 m	37.5 m	37.5 m	37.5 m	37.5 m
Distance to furnace or incinerator flue (meters)	N/A	N/A	N/A	N/A	N/A
Distance between monitors fulfilling a QA collocation requirement (meters).	N/A	N/A	N/A	N/A	N/A
Unrestricted airflow (degrees around probe/inlet or percentage of monitoring path)	360	360	360	360	360
Probe material for reactive gases NO/NO <sub>2</sub> /NO <sub>y</sub> , SO <sub>2</sub> , O <sub>3</sub> ; PAMS: VOCs, Carbonyls (e.g. Pyrex, stainless steel, Teflon)	Teflon/Pyrex with Borosilicate	N/A	N/A	Teflon/Pyrex with Borosilicate	N/A
Residence time for reactive gases NO/NO <sub>2</sub> /NO <sub>y</sub> , SO <sub>2</sub> , O <sub>3</sub> ; PAMS: VOCs, Carbonyls (seconds)	12.3	N/A	N/A	14.2	N/A
Frequency of one-point QC check for gaseous instruments	Daily	N/A	N/A	Daily	N/A
Frequency of flow rate verification for manual PM samplers, including Pb samplers (routine checks)	N/A	N/A	Monthly	N/A	N/A
Frequency of flow rate verification for automated PM analyzers (routine checks)	N/A	Bi-weekly	N/A	N/A	N/A
For low volume PM instruments (flow rate < 200 liters/minute), is any PM instrument within 1 m of the lovol? If yes, please list distance (meters) and instrument(s).	N/A	No	N/A	N/A	N/A

<b>Pollutant</b>	<b>Ozone</b>	<b>PM2.5</b>	<b>PM10</b>	<b>NO<sub>2</sub></b>	<b>Meteorology</b>
For high volume PM instrument (flow rate > 200 liters/minute), is any PM instrument within 2m of the hivol? If yes, please list distance (meters) and instrument(s).	N/A	N/A	No	N/A	N/A
Date of Annual Performance Evaluation conducted in the past calendar year for gaseous parameters (MM/DD/YYYY)	11/27/17	N/A	N/A	11/27/17	N/A
Date of two semi-annual flow rate audits conducted in the past calendar year for PM monitors (MM/DD/YYYY, MM/DD/YYYY)	N/A	05/17/17, 11/27/17	05/17/17, 11/27/17	N/A	N/A
Changes planned within the next 18 months (Y/N)	N	N	N	N	N

<b>Site Name</b>	<b>Merced - M St</b>
<b>AQS ID (XX-XXX-XXXX)</b>	06-047-2510
<b>Representative statistical area Name (i.e. MSA, CBSA, other)</b>	Merced
<b>County</b>	Merced
<b>Collecting (Operating) Agency</b>	SJVAPCD
<b>Analytical Lab (i.e. weigh lab, toxics lab, other)</b>	CARB
<b>Reporting Agency</b>	CARB: PM10 FRM and PM2.5 FRM
<b>Site Start Date</b>	04/01/1999
<b>Pollutant Parameters</b>	PM10 FRM, PM2.5 FRM
<b>Meteorological Parameters</b>	None
<b>Address</b>	2334 M Street, Merced, CA 95340
<b>GPS Coordinates (decimal degrees)</b>	37.3086 N, -120.4800 W
<b>Distance to roadways (meters)</b>	55 m (northwest)
<b>Traffic Count/Year</b>	51,000/2014 (Traffic count for nearest roads: R Street/Rte 99, Source: Caltrans 2016 AADT)
<b>Groundcover (e.g. paved, vegetative, dirt, sand, gravel)</b>	Paved, gravel

<b>Merced – M St (1)</b>		
<b>Pollutant</b>	<b>PM2.5</b>	<b>PM10</b>
Parameter code	88101	81102
Spatial scale	N	N
Site type	HC, PE	HC, PE
Basic monitoring objective(s)	NC, RS	NC, RS
Monitor type	SLAMS	SLAMS
Network affiliation(s), if applicable (a monitor may have none, one, or multiple)	None	None
FRM/FEM/ARM/Other	FRM	FRM
POC	1	1
Primary / QA Collocated / Other (provide for all PM <sub>2.5</sub> , PM <sub>10</sub> , PM <sub>10-2.5</sub> , Pb and NO <sub>2</sub> monitors. Non-PM, Pb, NO <sub>2</sub> monitors should be listed as "N/A".)	Primary	Primary
Is it suitable for comparison against the annual PM <sub>2.5</sub> ? (Y/N)	Y	N/A
Instrument manufacturer and model	Thermo-Partisol 2025i	ECOTECH Hi-Vol 3000
Analysis method	Gravimetric	Gravimetric
Method code	145	162
Monitoring start date (MM/DD/YYYY)	04/01/1999	4/01/1999
Required sampling frequency (e.g. 1:3 excluding exceptional events/1:1 including exceptional events)	1:3	1:6
Sampling season (MM/DD - MM/DD)	1/1 -12/31	1/1 – 12/31
Probe height (meters)	8.4 m	8.4 m
Distance from supporting structure (meters)	2.05 m	1.7 m
Distance from obstructions on roof. Include horizontal distance + vertical height above probe for obstructions nearby. (meters)	N/A	N/A
Distance from obstructions not on roof. Include horizontal distance + vertical height above probe for obstructions nearby. (meters)	N/A	N/A
Distance from trees (meters)	50 m east	50 m east
Distance to furnace or incinerator flue (meters)	42 m	38 m

<b>Pollutant</b>	<b>PM2.5</b>	<b>PM10</b>
Distance between monitors fulfilling a QA collocation requirement (meters).	N/A	N/A
Unrestricted airflow (degrees around probe/inlet or percentage of monitoring path)	360	360
Probe material for reactive gases NO/NO <sub>2</sub> /NO <sub>y</sub> , SO <sub>2</sub> , O <sub>3</sub> ; PAMS: VOCs, Carbonyls (e.g. Pyrex, stainless steel, Teflon)	N/A	N/A
Residence time for reactive gases NO/NO <sub>2</sub> /NO <sub>y</sub> , SO <sub>2</sub> , O <sub>3</sub> ; PAMS: VOCs, Carbonyls (seconds)	N/A	N/A
Frequency of one-point QC check for gaseous instruments	N/A	N/A
Frequency of flow rate verification for manual PM samplers, including Pb samplers (routine checks)	Bi-weekly	Monthly
Frequency of flow rate verification for automated PM analyzers (routine checks)	N/A	N/A
For low volume PM instruments (flow rate < 200 liters/minute), is any PM instrument within 1 m of the lovol? If yes, please list distance (meters) and instrument(s).	No	N/A
For high volume PM instrument (flow rate > 200 liters/minute), is any PM instrument within 2m of the hivol? If yes, please list distance (meters) and instrument(s).	N/A	No
Date of Annual Performance Evaluation conducted in the past calendar year for gaseous parameters (MM/DD/YYYY)	N/A	N/A
Date of two semi-annual flow rate audits conducted in the past calendar year for PM monitors (MM/DD/YYYY, MM/DD/YYYY)	05/01/17, 11/28/17	05/01/17, 11/28/17
Changes planned within the next 18 months (Y/N)	N	N

<b>Site Name</b>	<b>Merced - Coffee</b>
<b>AQS ID (XX-XXX-XXXX)</b>	06-047-0003
<b>Representative statistical area Name (i.e. MSA, CBSA, other)</b>	Merced
<b>County</b>	Merced
<b>Collecting (Operating) Agency</b>	SJVAPCD
<b>Analytical Lab (i.e. weigh lab, toxics lab, other)</b>	N/A
<b>Reporting Agency</b>	SJVAPCD
<b>Site Start Date</b>	10/1/1991
<b>Pollutant Parameters</b>	Ozone, PM2.5 FEM, NO2
<b>Meteorological Parameters</b>	Wind speed, wind direction, outdoor temperature
<b>Address</b>	385 S. Coffee St., Merced, CA 95340
<b>GPS Coordinates (decimal degrees)</b>	37.2816 N, -120.4340 W
<b>Distance to roadways (meters)</b>	15 m (east)
<b>Traffic Count/Year</b>	42,500/2014 (Traffic count for nearest roads: Childs Avenue/Rte 99, Source: Caltrans 2016 AADT)
<b>Groundcover (e.g. paved, vegetative, dirt, sand, gravel)</b>	Vegetative, dirt and gravel

Merced – Coffee (1)				
Pollutant	Ozone	PM2.5	NO <sub>2</sub>	Meteorology
Parameter code	44201	88101	42602	Many
Spatial scale	N	N	N	R
Site type	HC, PE	PE	PE	GB
Basic monitoring objective(s)	NC, RS, TP	NC, RS, TP	NC, RS, TP	RS, TP
Monitor type	SLAMS	SLAMS	SLAMS	Other
Network affiliation(s), if applicable (a monitor may have none, one, or multiple)	None	None	None	None
FRM/FEM/ARM/Other	FEM	FEM	FEM	Other
POC	1	3	1	Many
Primary / QA Collocated / Other (provide for all PM <sub>2.5</sub> , PM <sub>10</sub> , PM <sub>10-2.5</sub> , Pb and NO <sub>2</sub> monitors. Non-PM, Pb, NO <sub>2</sub> monitors should be listed as "N/A".)	N/A	Primary	N/A	Other
Is it suitable for comparison against the annual PM <sub>2.5</sub> ? (Y/N)	N/A	Y	N/A	N/A
Instrument manufacturer and model	Teledyne T400	MET One BAM 1020	Teledyne T200	ITP- Hy-Cal 512AA3B, OT- Met One 060A-2, WD- Met One 020C, WS-Met One 010C
Analysis method	UV	Beta Attenuation	CL	Many
Method code	087	170	099	Many
Monitoring start date (MM/DD/YYYY)	10/01/1991	10/19/2009	10/01/1991	10/01/1991
Required sampling frequency (e.g. 1:3 excluding exceptional events/1:1 including exceptional events)	Hourly	Hourly	Hourly	Hourly
Sampling season (MM/DD - MM/DD)	01/01 – 12/31	01/01 – 12/31	01/01 – 12/31	01/01 – 12/31
Probe height (meters)	5.4 m	5.4 m	5.4 m	7.6 m
Distance from supporting structure (meters)	1.9 m	1.9 m	1.9 m	4.1 m
Distance from obstructions on roof. Include horizontal distance + vertical height above probe for obstructions nearby. (meters)	N/A	N/A	N/A	N/A
Distance from obstructions not on roof. Include horizontal distance + vertical height above probe for obstructions nearby. (meters)	N/A	N/A	N/A	N/A
Distance from trees (meters)	13.5 m	14.0 m	13.5 m	13.5 m



Pollutant	Ozone	PM2.5	NO <sub>2</sub>	Meteorology
Distance to furnace or incinerator flue (meters)	N/A	N/A	N/A	N/A
Distance between monitors fulfilling a QA collocation requirement (meters).	N/A	N/A	N/A	N/A
Unrestricted airflow (degrees around probe/inlet or percentage of monitoring path)	360	360	360	360
Probe material for reactive gases NO/NO <sub>2</sub> /NO <sub>y</sub> , SO <sub>2</sub> , O <sub>3</sub> ; PAMS: VOCs, Carbonyls (e.g. Pyrex, stainless steel, Teflon)	Teflon/Pyrex with Borosilicate	N/A	Teflon/Pyrex with Borosilicate	N/A
Residence time for reactive gases NO/NO <sub>2</sub> /NO <sub>y</sub> , SO <sub>2</sub> , O <sub>3</sub> ; PAMS: VOCs, Carbonyls (seconds)	11.9	N/A	12.7	N/A
Frequency of one-point QC check for gaseous instruments	Daily	N/A	Daily	N/A
Frequency of flow rate verification for manual PM samplers, including Pb samplers (routine checks)	N/A	N/A	N/A	N/A
Frequency of flow rate verification for automated PM analyzers (routine checks)	N/A	Bi-weekly	N/A	N/A
For low volume PM instruments (flow rate < 200 liters/minute), is any PM instrument within 1 m of the hivol? If yes, please list distance (meters) and instrument(s).	N/A	No	N/A	N/A
For high volume PM instrument (flow rate > 200 liters/minute), is any PM instrument within 2m of the hivol? If yes, please list distance (meters) and instrument(s).	N/A	N/A	N/A	N/A
Date of Annual Performance Evaluation conducted in the past calendar year for gaseous parameters (MM/DD/YYYY)	11/28/17	N/A	11/28/17	N/A
Date of two semi-annual flow rate audits conducted in the past calendar year for PM monitors (MM/DD/YYYY, MM/DD/YYYY)	N/A	05/17/17, 11/28/17	N/A	N/A
Changes planned within the next 18 months (Y/N)	N	N	N	N

<b>Site Name</b>	<b>Madera - City</b>
<b>AQS ID (XX-XXX-XXXX)</b>	06-039-2010
<b>Representative statistical area Name (i.e. MSA, CBSA, other)</b>	Madera
<b>County</b>	Madera
<b>Collecting (Operating) Agency</b>	SJVAPCD
<b>Analytical Lab (i.e. weigh lab, toxics lab, other)</b>	CARB: PM2.5 FRM
<b>Reporting Agency</b>	SJVAPCD
<b>Site Start Date</b>	6/1/2010
<b>Pollutant Parameters</b>	Ozone, PM10 FEM, PM2.5 FEM, PM2.5 FRM
<b>Meteorological Parameters</b>	Wind speed, wind direction, outdoor temperature, relative humidity, barometric pressure, solar radiation.
<b>Address</b>	28261 Avenue 14, Madera, CA 93638
<b>GPS Coordinates (decimal degrees)</b>	36.9532 N, -120.0342 W
<b>Distance to roadways (meters)</b>	70 m (south)
<b>Traffic Count/Year</b>	386/2017 (Traffic count for nearest roads: Avenue 14 west of Road 29, westbound trips per hour in 24 hours. Source: Madera County Transportation Commission 2017 Traffic Volumes Report.)
<b>Groundcover (e.g. paved, vegetative, dirt, sand, gravel)</b>	Paved, dirt, and vegetative

Madera – City (1)								
Pollutant	Ozone	PM2.5	PM2.5	PM2.5	PM10 LC	PM10 STP	PM10 STP	Meteorology
Parameter code	44201	88101	88101	88101	85101	81102	81102	Many
Spatial scale	N	N	N	N	N	N	N	N
Site type	HC, GB	HC, QA	PE	PE	PE	PE	PE	GB
Basic monitoring objective(s)	NC, RS, TP	NC, RS,	NC, RS, TP	NC, RS, TP	RS, TP	NC, RS, TP	NC, RS, TP	RS, TP
Monitor type	SLAMS	SLAMS	SLAMS	SLAMS	SLAMS	SLAMS	SLAMS	Other
Network affiliation(s), if applicable (a monitor may have none, one, or multiple)	None	None	None	None	None	None	None	None
FRM/FEM/ARM/Other	FEM	FRM	FEM	FEM	FEM	FEM	FEM	Other
POC	1	1	3	3	3	3	3	1
Primary / QA Collocated / Other (provide for all PM <sub>2.5</sub> , PM <sub>10</sub> , PM <sub>10-2.5</sub> , Pb and NO <sub>2</sub> monitors. Non-PM, Pb, NO <sub>2</sub> monitors should be listed as "N/A".)	N/A	QA Collocated	Primary	Primary	Other	Other	Primary	Other
Is it suitable for comparison against the annual PM <sub>2.5</sub> ? (Y/N)	N/A	Y	Y	Y	N/A	N/A	N/A	N/A
Instrument manufacturer and model	TAPI 400E IZS	Thermo Partisol 2025i	MET One BAM 1020	Teledyne 602	Teledyne 602	Teledyne 602	Thermo TEOM 1400	ITP- Hy-Cal 512AA3B, OT- Met One 060A-2, BP- Met One 092, WD- Met One 020C, WS-Met One 010C
Analysis method	UV	Gravimetric	Beta Attenuation	Beta Attenuation	Beta Attenuation	Beta Attenuation	Tapered Element	Many
Method code	087	145	170	205	204	204	079	Many
Monitoring start date (MM/DD/YYYY)	06/01/2010	02/17/2014	06/01/2010	12/01/2017	12/01/2017	12/01/2017	06/01/2010	06/01/2010

Pollutant	Ozone	PM2.5	PM2.5	PM2.5	PM10 LC	PM10 STP	PM10 STP	Meteorology
Required sampling frequency (e.g. 1:3 excluding exceptional events/1:1 including exceptional events)	Hourly	1:12	Hourly	Hourly	Hourly	Hourly	Hourly	Hourly
Sampling season (MM/DD - MM/DD)	01/01 – 12/31	01/01 – 12/31	01/01 – 12/31	01/01 - 12/31	01/01 - 12/31	01/01 - 12/31	01/01 – 12/31	01/01 – 12/31
Probe height (meters)	5.1 m	5.1 m	4.7 m	4.4 m	5.0 m	6.35 m	4.6 m	10 m
Distance from supporting structure (meters)	2 m	2.1 m	1.8 m	1.8 m	2.4 m	2.4 m	1.8 m	7 m
Distance from obstructions not on roof. Include horizontal distance + vertical height above probe for obstructions nearby. (meters)	N/A	N/A	N/A	N/A	N/A	N/A	N/A	N/A
Distance from trees (meters)	14.5 m	16.5 m	16.5 m	15 m	15 m	15 m	13 m	14.5 m
Distance to furnace or incinerator flue (meters)	53m	53m	52m	53m	53m	53m	54m	N/A
Distance between monitors fulfilling a QA collocation requirement (meters).	N/A	N/A	N/A	N/A	N/A	N/A	N/A	N/A
Unrestricted airflow (degrees around probe/inlet or percentage of monitoring path)	360	360	360	360	360	360	360	360
Probe material for reactive gases NO/NO <sub>2</sub> /NO <sub>y</sub> , SO <sub>2</sub> , O <sub>3</sub> ; PAMS: VOCs, Carbonyls (e.g. Pyrex, stainless steel, Teflon)	Teflon/Pyrex with Borosilicate	N/A	N/A	N/A	N/A	N/A	N/A	N/A

Pollutant	Ozone	PM2.5	PM2.5	PM2.5	PM10 LC	PM10 STP	PM10 STP	Meteorology
Residence time for reactive gases NO/NO <sub>2</sub> /NO <sub>y</sub> , SO <sub>2</sub> , O <sub>3</sub> ; NPAMS: VOCs, Carbonyls (seconds)	4.9	N/A	N/A	N/A	N/A	N/A	N/A	N/A
Frequency of one-point QC check for gaseous instruments	Daily	N/A	N/A	N/A	N/A	N/A	N/A	N/A
Frequency of flow rate verification for manual PM samplers, including Pb samplers (routine checks)	N/A	Monthly	N/A	N/A	N/A	N/A	N/A	N/A
Frequency of flow rate verification for automated PM analyzers (routine checks)	N/A	N/A	Bi-Weekly	Bi-Weekly	Bi-Weekly	Bi-Weekly	Bi-Weekly	N/A
For low volume PM instruments (flow rate < 200 liters/minute), is any PM instrument within 1 m of the lovol? If yes, please list distance (meters) and instrument(s).	N/A	No	No	No	No	No	No	N/A
For high volume PM instrument (flow rate > 200 liters/minute), is any PM instrument within 2m of the hivol? If yes, please list distance (meters) and instrument(s).	N/A	N/A	N/A	N/A	N/A	N/A	N/A	N/A

Pollutant	Ozone	PM2.5	PM2.5	PM2.5	PM10 LC	PM10 STP	PM10 STP	Meteorology
Date of Annual Performance Evaluation conducted in the past calendar year for gaseous parameters (MM/DD/YYYY)	11/13/17	N/A	N/A	N/A	N/A	N/A	N/A	N/A
Date of two semi-annual flow rate audits conducted in the past calendar year for PM monitors (MM/DD/YYYY, MM/DD/YYYY)	N/A	5/15/17, 11/13/17	5/15/17, 11/13/17	5/15/17, 11/13/17	5/15/17, 11/13/17	5/15/17, 11/13/17	5/15/17, 11/13/17	N/A
Changes planned within the next 18 months (Y/N)	N	N	Shut down 12/1/17	Change inlet tube height	Change inlet tube height	Change inlet tube height	Shut down 12/1/17	N

<b>Site Name</b>	<b>Madera – Pump Yard</b>
<b>AQS ID (XX-XXX-XXXX)</b>	06-039-0004
<b>Representative statistical area Name (i.e. MSA, CBSA, other)</b>	Madera
<b>County</b>	Madera
<b>Collecting (Operating) Agency</b>	SJVAPCD
<b>Analytical Lab (i.e. weigh lab, toxics lab, other)</b>	Varies based on which laboratory is contracted with the SJVAPCD.
<b>Reporting Agency</b>	SJVAPCD
<b>Site Start Date</b>	07/01/1997
<b>Pollutant Parameters</b>	Ozone, NO <sub>2</sub> , Speciated VOC, NMH
<b>Meteorological Parameters</b>	Wind speed, wind direction, outdoor temperature, relative humidity, barometric pressure, solar radiation
<b>Address</b>	Avenue 8 and Road 29 ½, Madera, CA 93637
<b>GPS Coordinates (decimal degrees)</b>	36.867125 N, -120.010158 W
<b>Distance to roadways (meters)</b>	20 m (west)
<b>Traffic Count/Year</b>	2,980/2017 (Traffic count for nearest roads: Avenue 7 west of Rte 99, westbound trips per hour in 24 hours. Source: Madera County Transportation Commission 2017 Traffic Volumes Report.)
<b>Groundcover (e.g. paved, vegetative, dirt, sand, gravel)</b>	Dirt, paved

Madera – Pump Yard (1)					
Pollutant	Ozone	NO <sub>2</sub>	Speciated VOC	NMH	Meteorology
Parameter code	44201	42602	Many	43102	Many
Spatial scale	N	N	N	N	R
Site type	HC, GB	PE	PE	PE	GB
Basic monitoring objective(s)	NC, RS, TP	NC, RS, TP	RS	RS	RS, TP
Monitor type	SLAMS	SLAMS	Other	Other	Other
Network affiliation(s), if applicable (a monitor may have none, one, or multiple)	PAMS	PAMS	PAMS	PAMS	PAMS
FRM/FEM/ARM/Other	FEM	FEM	Other	Other	Other
POC	1	1	1	1	Many
Primary / QA Collocated / Other (provide for all PM <sub>2.5</sub> , PM <sub>10</sub> , PM <sub>10-2.5</sub> , Pb and NO <sub>2</sub> monitors. Non-PM, Pb, NO <sub>2</sub> monitors should be listed as "N/A".)	N/A	N/A	N/A	N/A	Other
Is it suitable for comparison against the annual PM <sub>2.5</sub> ? (Y/N)	N/A	N/A	N/A	N/A	N/A
Instrument manufacturer and model	Teledyne 400E	Teledyne T200	Xontech 910A	Synspec Alpha 115	ITP- Hamp.Control 125-50, OT- Met One 060A-2, BP- Met One 092, RH- Vaisala HMP110A, SRD- Epply Mod. 8-48, WD- Met One 020C, WS-Met One 010C
Analysis method	UV	CL	GC	GC	Many
Method code	087	099	164	011	Many
Monitoring start date (MM/DD/YYYY)	07/01/1997	07/01/1997	07/01/1997	07/01/1997	07/01/1997
Required sampling frequency (e.g. 1:3 excluding exceptional events/1:1 including exceptional events)	Hourly	Hourly	1:3	Hourly	Hourly
Sampling season (MM/DD - MM/DD)	01/01 – 12/31	01/01 – 12/31	06/01 – 8/31	01/01 – 12/31	01/01 – 12/31
Probe height (meters)	5.8 m	5.8 m	5.8 m	5.8 m	10 m
Distance from supporting structure (meters)	2 m	2 m	2 m	2 m	8.2 m



Pollutant	Ozone	NO <sub>2</sub>	Speciated VOC	NMH	Meteorology
Distance from obstructions on roof. Include horizontal distance + vertical height above probe for obstructions nearby. (meters)	N/A	N/A	N/A	N/A	N/A
Distance from obstructions not on roof. Include horizontal distance + vertical height above probe for obstructions nearby. (meters)	Horiz. 20 m, Vert 0 m above	Horiz. 20 m, Vert 0 m above	Horiz. 20 m, Vert 0 m above	Horiz. 20 m, Vert 0 m above	Horiz. 20 m, Vert 0 m above
Distance from trees (meters)	40.5 m	40.5 m	40.5 m	40.5 m	40.5 m
Distance to furnace or incinerator flue (meters)	N/A	N/A	N/A	N/A	N/A
Distance between monitors fulfilling a QA collocation requirement (meters).	N/A	N/A	N/A	N/A	N/A
Unrestricted airflow (degrees around probe/inlet or percentage of monitoring path)	360	360	360	360	360
Probe material for reactive gases NO/NO <sub>2</sub> /NO <sub>y</sub> , SO <sub>2</sub> , O <sub>3</sub> ; PAMS: VOCs, Carbonyls (e.g. Pyrex, stainless steel, Teflon)	Teflon/Pyrex with Borosilicate	Teflon/Pyrex with Borosilicate	Stainless steel	Stainless steel	N/A
Residence time for reactive gases NO/NO <sub>2</sub> /NO <sub>y</sub> , SO <sub>2</sub> , O <sub>3</sub> ; PAMS: VOCs, Carbonyls (seconds)	11.97	12.63	11.41	11.41	N/A
Frequency of one-point QC check for gaseous instruments	Daily	Daily	Daily	Daily	N/A
Frequency of flow rate verification for manual PM samplers, including Pb samplers (routine checks)	N/A	N/A	N/A	N/A	N/A
Frequency of flow rate verification for automated PM analyzers (routine checks)	N/A	N/A	N/A	N/A	N/A
For low volume PM instruments (flow rate < 200 liters/minute), is any PM instrument within 1 m of the level? If yes, please list distance (meters) and instrument(s).	N/A	N/A	N/A	N/A	N/A

Pollutant	Ozone	NO <sub>2</sub>	Speciated VOC	NMH	Meteorology
For high volume PM instrument (flow rate > 200 liters/minute), is any PM instrument within 2m of the hivol? If yes, please list distance (meters) and instrument(s).	N/A	N/A	N/A	N/A	N/A
Date of Annual Performance Evaluation conducted in the past calendar year for gaseous parameters (MM/DD/YYYY)	11/14/17	11/14/17	N/A	N/A	N/A
Date of two semi-annual flow rate audits conducted in the past calendar year for PM monitors (MM/DD/YYYY, MM/DD/YYYY)	N/A	N/A	N/A	N/A	N/A
Changes planned within the next 18 months (Y/N)	N	N	N	N	N

<b>Site Name</b>	<b>Tranquillity</b>
<b>AQS ID (XX-XXX-XXXX)</b>	06-019-2009
<b>Representative statistical area Name (i.e. MSA, CBSA, other)</b>	Fresno
<b>County</b>	Fresno
<b>Collecting (Operating) Agency</b>	SJVAPCD
<b>Analytical Lab (i.e. weigh lab, toxics lab, other)</b>	N/A
<b>Reporting Agency</b>	SJVAPCD
<b>Site Start Date</b>	09/01/2009
<b>Pollutant Parameters</b>	Ozone, PM2.5 FEM
<b>Meteorological Parameters</b>	Wind speed, wind direction, outdoor temperature, barometric pressure
<b>Address</b>	32650 W. Adams, Tranquillity, CA 93668
<b>GPS Coordinates (decimal degrees)</b>	36.6008 N, -120.3822 W
<b>Distance to roadways (meters)</b>	200m (south)
<b>Traffic Count/Year</b>	2,292/2018 (Raw traffic count for nearest roads: Northbound Derrick Avenue between W. Nebraska Avenue and West Mountain View Avenue, Source: Fresno COG Traffic Counts, 2007-2018 Kittelson & Associates, Inc.)
<b>Groundcover (e.g. paved, vegetative, dirt, sand, gravel)</b>	Dirt, vegetative

<b>Tranquillity (1)</b>			
<b>Pollutant</b>	<b>Ozone</b>	<b>PM2.5</b>	<b>Meteorology</b>
Parameter code	44201	88101	Many
Spatial scale	U	U	U
Site type	PE	PE	PE
Basic monitoring objective(s)	NC, RS, TP	NC, RS, TP	TP
Monitor type	SLAMS	SLAMS	Other
Network affiliation(s), if applicable (a monitor may have none, one, or multiple)	None	None	None
FRM/FEM/ARM/Other	FEM	FEM	Other
POC	1	3	1
Primary / QA Collocated / Other (provide for all PM <sub>2.5</sub> , PM <sub>10</sub> , PM <sub>10-2.5</sub> , Pb and NO <sub>2</sub> monitors. Non-PM, Pb, NO <sub>2</sub> monitors should be listed as "N/A".)	Primary	Primary	Other
Is it suitable for comparison against the annual PM <sub>2.5</sub> ? (Y/N)	N/A	Y	N/A
Instrument manufacturer and model	Teledyne 400E (IZS)	MET One BAM 1020	ITP- Hy-Cal 512AA3B, OT- Met One 060A-2, BP- Met One 092, WD- Met One 020C, WS-Met One 010C
Analysis method	UV	Beta attenuation	Many
Method code	087	170	Many
Monitoring start date (MM/DD/YYYY)	10/30/2009	10/30/2009	10/30/2009
Required sampling frequency (e.g. 1:3 excluding exceptional events/1:1 including exceptional events)	Hourly	Hourly	Hourly
Sampling season (MM/DD - MM/DD)	01/01 – 12/31	01/01 – 12/31	01/01 – 12/31
Probe height (meters)	4.6 m	4.9 m	10.6m
Distance from supporting structure (meters)	1.8 m	2.1 m	0 m
Distance from obstructions on roof. Include horizontal distance + vertical height above probe for obstructions nearby. (meters)	N/A	N/A	N/A
Distance from obstructions not on roof. Include horizontal distance + vertical height above probe for obstructions nearby. (meters)	82.8 m	76.8 m	76.7m
Distance from trees (meters)	63.7 m	66.1 m	63.7m
Distance to furnace or incinerator flue (meters)	N/A	N/A	N/A

Pollutant	Ozone	PM2.5	Meteorology
Distance between monitors fulfilling a QA collocation requirement (meters).	N/A	N/A	N/A
Unrestricted airflow (degrees around probe/inlet or percentage of monitoring path)	359	359	360
Probe material for reactive gases NO/NO <sub>2</sub> /NO <sub>y</sub> , SO <sub>2</sub> , O <sub>3</sub> ; PAMS: VOCs, Carbonyls (e.g. Pyrex, stainless steel, Teflon)	Teflon/Pyrex with Borosilicate	N/A	N/A
Residence time for reactive gases NO/NO <sub>2</sub> /NO <sub>y</sub> , SO <sub>2</sub> , O <sub>3</sub> ; PAMS: VOCs, Carbonyls (seconds)	3.6	N/A	N/A
Frequency of one-point QC check for gaseous instruments	Daily	N/A	N/A
Frequency of flow rate verification for manual PM samplers, including Pb samplers (routine checks)	N/A	N/A	N/A
Frequency of flow rate verification for automated PM analyzers (routine checks)	N/A	Bi-Weekly	N/A
For low volume PM instruments (flow rate < 200 liters/minute), is any PM instrument within 1 m of the hivol? If yes, please list distance (meters) and instrument(s).	N/A	No	N/A
For high volume PM instrument (flow rate > 200 liters/minute), is any PM instrument within 2m of the hivol? If yes, please list distance (meters) and instrument(s).	N/A	No	N/A
Date of Annual Performance Evaluation conducted in the past calendar year for gaseous parameters (MM/DD/YYYY)	11/16/17	N/A	N/A
Date of two semi-annual flow rate audits conducted in the past calendar year for PM monitors (MM/DD/YYYY, MM/DD/YYYY)	N/A	05/16/17, 11/16/17	N/A
Changes planned within the next 18 months (Y/N)	N	N	N

<b>Site Name</b>	<b>Fresno – Sierra Sky Park</b>
<b>AQS ID (XX-XXX-XXXX)</b>	06-019-0242
<b>Representative statistical area Name (i.e. MSA, CBSA, other)</b>	Fresno
<b>County</b>	Fresno
<b>Collecting (Operating) Agency</b>	SJVAPCD
<b>Analytical Lab (i.e. weigh lab, toxics lab, other)</b>	N/A
<b>Reporting Agency</b>	SJVAPCD
<b>Site Start Date</b>	7/1/1986
<b>Pollutant Parameters</b>	Ozone, NO2
<b>Meteorological Parameters</b>	Wind speed, wind direction, outdoor temperature
<b>Address</b>	4508 Chenault Ave., Fresno, CA 93722
<b>GPS Coordinates (decimal degrees)</b>	36.8405 N, -119.8740 W
<b>Distance to roadways (meters)</b>	12m (west)
<b>Traffic Count/Year</b>	15,626 / 2018 (Raw traffic count in a 24-hour period for nearest roads: Spruce Avenue east of Milburn Avenue. Source: Fresno COG Traffic Counts, 2007-2018 Kittelson & Associates, Inc.)
<b>Groundcover (e.g. paved, vegetative, dirt, sand, gravel)</b>	Gravel, dirt

Fresno – Sierra Sky Park (1)			
Pollutant	Ozone	NO <sub>2</sub>	Meteorology
Parameter code	44201	42602	Many
Spatial scale	N	N	N
Site type	HC, PE, RT	PE	GB
Basic monitoring objective(s)	NC, RS, TP	NC, RS, TP	RS, TP
Monitor type	SLAMS	SLAMS	Other
Network affiliation(s), if applicable (a monitor may have none, one, or multiple)	N/A	N/A	N/A
FRM/FEM/ARM/Other	FEM	FEM	Other
POC	1	1	1
Primary / QA Collocated / Other (provide for all PM <sub>2.5</sub> , PM <sub>10</sub> , PM <sub>10-2.5</sub> , Pb and NO <sub>2</sub> monitors. Non-PM, Pb, NO <sub>2</sub> monitors should be listed as "N/A".)	N/A	N/A	Other
Is it suitable for comparison against the annual PM <sub>2.5</sub> ? (Y/N)	N/A	N/A	N/A
Instrument manufacturer and model	Teledyne 400E	Teledyne T200	ITP- BA-512-A-A-3-B, OT- Met One 060A-2, WD- Met One 020C, WS- Met One 010C
Analysis method	UV	CL	Many
Method code	087	574	Many
Monitoring start date (MM/DD/YYYY)	07/01/1986	07/01/1986	07/01/1986
Required sampling frequency (e.g. 1:3 excluding exceptional events/1:1 including exceptional events)	Hourly	Hourly	Hourly
Sampling season (MM/DD - MM/DD)	01/01 – 12/31	01/01 – 12/31	01/01 – 12/31
Probe height (meters)	5.5 m	5.5 m	5.6 m
Distance from supporting structure (meters)	2.3 m	2.3 m	2.3 m
Distance from obstructions on roof. Include horizontal distance + vertical height above probe for obstructions nearby. (meters)	N/A	N/A	N/A
Distance from obstructions not on roof. Include horizontal distance + vertical height above probe for obstructions nearby. (meters)	N/A	N/A	N/A
Distance from trees (meters)	2.2 m	2.2 m	1.2 m

Pollutant	Ozone	NO <sub>2</sub>	Meteorology
Distance to furnace or incinerator flue (meters)	N/A	N/A	N/A
Distance between monitors fulfilling a QA collocation requirement (meters).	N/A	N/A	N/A
Unrestricted airflow (degrees around probe/inlet or percentage of monitoring path)	280	280	280
Probe material for reactive gases NO/NO <sub>2</sub> /NO <sub>y</sub> , SO <sub>2</sub> , O <sub>3</sub> ; PAMS: VOCs, Carbonyls (e.g. Pyrex, stainless steel, Teflon)	Teflon/Pyrex with Borosilicate	Teflon/Pyrex with Borosilicate	N/A
Residence time for reactive gases NO/NO <sub>2</sub> /NO <sub>y</sub> , SO <sub>2</sub> , O <sub>3</sub> ; PAMS: VOCs, Carbonyls (seconds)	12.33	12.99	N/A
Frequency of one-point QC check for gaseous instruments	Daily	Daily	N/A
Frequency of flow rate verification for manual PM samplers, including Pb samplers (routine checks)	N/A	N/A	N/A
Frequency of flow rate verification for automated PM analyzers (routine checks)	N/A	N/A	N/A
For low volume PM instruments (flow rate < 200 liters/minute), is any PM instrument within 1 m of the hivol? If yes, please list distance (meters) and instrument(s).	N/A	N/A	N/A
For high volume PM instrument (flow rate > 200 liters/minute), is any PM instrument within 2m of the hivol? If yes, please list distance (meters) and instrument(s).	N/A	N/A	N/A
Date of Annual Performance Evaluation conducted in the past calendar year for gaseous parameters (MM/DD/YYYY)	03/14/17	03/14/17	N/A
Date of two semi-annual flow rate audits conducted in the past calendar year for PM monitors (MM/DD/YYYY, MM/DD/YYYY)	N/A	N/A	N/A
Changes planned within the next 18 months (Y/N)	N	N	N



<b>Site name</b>	<b>Clovis – Villa</b>		
<b>AQS ID (XX-XXX-XXXX)</b>	06-019-5001		
<b>Representative statistical area Name (i.e. MSA, CBSA, other)</b>	Fresno		
<b>County</b>	Fresno		
<b>Collecting (Operating) Agency</b>	SJVAPCD		
<b>Analytical Lab (i.e. weigh lab, toxics lab, other)</b>	Varies based on which laboratory is contracted with the SJVAPCD: Speciated VOC	CARB: PM10 FRM, PM2.5 FRM	
<b>Reporting Agency</b>	SJVAPCD: PM2.5 FRM, PM2.5 FEM, PM10 FRM, PM10 FEM, Ozone, CO, NO <sub>2</sub> , NMH, Speciated VOC, Meteorology	CARB: PM10 FRM, PM2.5 FRM	SJVAPCD contracts out so Reporting lab varies from year to year: Speciated VOC
<b>Site Start Date</b>	09/01/1990		
<b>Pollutant Parameters</b>	Ozone, PM10 FRM, PM10 FEM, PM2.5 FEM, PM2.5 FRM, CO, NO <sub>2</sub> , NMH, Speciated VOC		
<b>Meteorological Parameters</b>	Wind speed, wind direction, outdoor temperature, relative humidity, barometric pressure, solar radiation		
<b>Address</b>	908 N. Villa Ave., Clovis CA 93612		
<b>GPS Coordinates (decimal degrees)</b>	36.8194 N, -119.7160 W		
<b>Distance to roadways (meters)</b>	260 m (east)		
<b>Traffic Count/Year</b>	13,890/2008 (Raw traffic count in a 24-hour period: Eastbound Bullard Avenue/Villa Avenue intersection) Source: Fresno COG Fresno County Regional Traffic Monitoring Report 2013 (new counts unavailable)		
<b>Groundcover (e.g. paved, vegetative, dirt, sand, gravel)</b>	Paved		

Clovis – Villa (1)							
Pollutant	Ozone	Ozone	PM10	PM2.5	PM10 LC	PM10 STP	PM2.5
Parameter Code	44201	44201	81102	88101	85101	81102	88101
Spatial scale	N	N	N	N	N	N	N
Site type	Max PEI, HC	Max PEI, HC	PE	HC	HC	HC	HC
Basic monitoring objective(s)	NC, RS, TP	NC, RS, TP	NC, RS	NC, RS, TP	RS, TP	NC, RS, TP	NC, RS
Monitor type	SLAMS	SLAMS	SLAMS	SLAMS	SLAMS	SLAMS	SLAMS
Network affiliation(s), if applicable (a monitor may have none, one, or multiple)	PAMS	PAMS	None	None	None	None	None
FRM/FEM/ARM/Other	FEM	FRM	FRM	FEM	FEM	FEM	FRM
POC	1	1	1	3	3	3	1
Primary / QA Collocated / Other (provide for all PM <sub>2.5</sub> , PM <sub>10</sub> , PM <sub>10-2.5</sub> , Pb and NO <sub>2</sub> monitors. Non-PM, Pb, NO <sub>2</sub> monitors should be listed as "N/A".)	N/A	N/A	Primary	Primary	Other	Other	QA Collocated
Is it suitable for comparison against the annual PM <sub>2.5</sub> ? (Y/N)	N/A	N/A	N/A	Y	N/A	N/A	Y
Instrument manufacturer and model	Teledyne 400 E	Teledyne API T265	Ecotech HiVol 3000	Teledyne 602	Teledyne 602	Teledyne 602	Thermo Partisol 2025i
Analysis method	UV	Chem.	Gravimetric	Beta Attenuation	Beta Attenuation	Beta Attenuation	Gravimetric
Method code	087	199	162	205	204	204	145
Monitoring start date (MM/DD/YYYY)	01/01/1990 – End Date: 04/30/2017	05/01/2017	04/01/2015	01/01/2017	01/01/2017	01/01/2017	09/06/2012
Required sampling frequency (e.g. 1:3 excluding exceptional events/1:1 including exceptional events)	Hourly	Hourly	1:6	Hourly	Hourly	Hourly	1:3
Sampling season (MM/DD - MM/DD)	01/01 - 12/31	01/01 - 12/31	01/01 - 12/31	01/01 - 12/31	01/01 - 12/31	01/01 - 12/31	01/01 - 12/31
Probe height (meters)	5.66 m	5.66 m	5.5 m	5.99 m	6.35 m	6.35 m	6.0 m
Distance from supporting structure (meters)	1.85 m	1.85 m	1.6 m	1.85 m	2.21 m	2.21 m	2m

Pollutant	Ozone	Ozone	PM10	PM2.5	PM10 LC	PM10 STP	PM2.5
Distance from obstructions on roof. Include horizontal distance + vertical height above probe for obstructions nearby. (meters)	N/A	N/A	N/A	N/A	N/A	N/A	N/A
Distance from obstructions not on roof. Include horizontal distance + vertical height above probe for obstructions nearby. (meters)	N/A	N/A	N/A	N/A	N/A	N/A	N/A
Distance from trees (meters)	15 m	15 m	15 m	17.5 m	17.5 m	17.5 m	37.5 m
Distance to furnace or incinerator flue (meters)	N/A	N/A	N/A	N/A	N/A	N/A	N/A
Distance between monitors fulfilling a QA collocation requirement (meters).	N/A	N/A	N/A	2.1 m	2.1 m	2.1 m	2.5
Unrestricted airflow (degrees around probe/inlet or percentage of monitoring path)	360	360	355	360	360	360	360
Probe material for reactive gases NO/NO <sub>2</sub> /NO <sub>y</sub> , SO <sub>2</sub> , O <sub>3</sub> ; PAMS: VOCs, Carbonyls (e.g. Pyrex, stainless steel, Teflon)	Teflon/Pyrex with Borosilicate	Teflon/Pyrex with Borosilicate	N/A	N/A	N/A	N/A	N/A
Residence time for reactive gases NO/NO <sub>2</sub> /NO <sub>y</sub> , SO <sub>2</sub> , O <sub>3</sub> ; PAMS: VOCs, Carbonyls (seconds)	8.2	5.08	N/A	N/A	N/A	N/A	N/A
For low volume PM instruments (flow rate < 200 liters/minute), is any PM instrument within 1 m of the lovol? If yes, please list distance (meters) and instrument(s).	N/A	N/A	No	No	No	No	No
For high volume PM instrument (flow rate > 200 liters/minute), is any PM instrument within 2m of the hivol? If yes, please list distance (meters) and instrument(s).	N/A	N/A	No	No	No	No	No
Frequency of flow rate verification for manual PM samplers, including Pb samplers (routine checks)	N/A	N/A	Monthly	N/A	N/A	N/A	Monthly

Pollutant	Ozone	Ozone	PM10	PM2.5	PM10 LC	PM10 STP	PM2.5
Frequency of flow rate verification for automated PM analyzers (routine checks)	N/A	N/A	N/A	Bi-weekly	Bi-weekly	Bi-weekly	N/A
Frequency of one-point QC check for gaseous instruments	Daily	Daily	N/A	N/A	N/A	N/A	N/A
Date of Annual Performance Evaluation conducted in the past calendar year for gaseous parameters (MM/DD/YYYY)	03/16/17	03/16/17	N/A	N/A	N/A	N/A	N/A
Date of two semi-annual flow rate audits conducted in the past calendar year for PM monitors (MM/DD/YYYY, MM/DD/YYYY)	N/A	N/A	03/16/17 09/19/17	03/16/17, 09/19/17	03/16/17, 09/19/17	03/16/17, 09/19/17	03/16/17 09/19/17
Changes planned within the next 18 months (Y/N)	Was removed 4/30/17	N	N	N	N	N	N

## Clovis – Villa (2)

Pollutant	CO	NO <sub>2</sub>	Speciated VOC	NMH	Meteorology
Parameter code	42101	42602	Many	43102	Many
Spatial scale	N	N	N	N	R
Site type	Max PEI, PE	HC	PE	HC	Other
Basic monitoring objective(s)	NC, RS, TP	NC, RS, TP	RS	RS	RS, TP
Monitor type	SLAMS	SLAMS	Other	Other	Other
Network affiliation(s), if applicable (a monitor may have none, one, or multiple)	PAMS	PAMS	PAMS	PAMS	PAMS
FRM/FEM/ARM/Other	FEM	FEM	Other	Other	Other
POC	1	1	1	1	1
Primary / QA Collocated / Other (provide for all PM <sub>2.5</sub> , PM <sub>10</sub> , PM <sub>10-2.5</sub> , Pb and NO <sub>2</sub> monitors. Non-PM, Pb, NO <sub>2</sub> monitors should be listed as "N/A".)	N/A	N/A	N/A	N/A	Other
Is it suitable for comparison against the annual PM <sub>2.5</sub> ? (Y/N)	N/A	N/A	N/A	N/A	N/A

Pollutant	CO	NO <sub>2</sub>	Speciated VOC	NMH	Meteorology
Instrument manufacturer and model	Themo 48i	Teledyne T200	Xontech 910A / Xontech 925	Synpec Alpha 115	ITP- HY-CAL BA 512- A-A-3-B, OT- Met- One 060A-2, BP- Met- One 092, RH- VAISALA HMP45D, SRD- EPPLY Mod.8- 48, WD- Met-One 020C, WS- Met One 010C, BP- Met One 092
Analysis method	IR	Chem.	GC / UV Absorption	Flame Ionization	Many
Method code	554	099	177 / 202	011	Many
Monitoring start date (MM/DD/YYYY)	01/01/1990	01/01/2016	01/01/1990	01/01/1990	01/01/1990
Required sampling frequency (e.g. 1:3 excluding exceptional events/1:1 including exceptional events)	Hourly	Hourly	1:3	Hourly	Hourly
Sampling season (MM/DD - MM/DD)	01/01 – 12/31	01/01 – 12/31	06/01 – 08/31	01/01 – 12/31	01/01 – 12/31
Probe height (meters)	5.66 m	5.66 m	5.66 m	5.66 m	10 m
Distance from supporting structure (meters)	1.85 m	1.85 m	1.85 m	1.85 m	7.5 m
Distance from obstructions on roof. Include horizontal distance + vertical height above probe for obstructions nearby. (meters)	N/A	N/A	N/A	N/A	N/A
Distance from obstructions not on roof. Include horizontal distance + vertical height above probe for obstructions nearby. (meters)	N/A	N/A	N/A	N/A	29.5 m
Distance from trees (meters)	15 m	15 m	15 m	15 m	25.5 m
Distance to furnace or incinerator flue (meters)	16.0 m	16.0 m	13.5 m	16.0 m	N/A
Distance between monitors fulfilling a QA collocation requirement (meters).	N/A	N/A	N/A	N/A	N/A
Unrestricted airflow (degrees around probe/inlet or percentage of monitoring path)	360	360	360	360	360

Pollutant	CO	NO <sub>2</sub>	Speciated VOC	NMH	Meteorology
Probe material for reactive gases NO/NO <sub>2</sub> /NO <sub>y</sub> , SO <sub>2</sub> , O <sub>3</sub> ; PAMS: VOCs, Carbonyls (e.g. Pyrex, stainless steel, Teflon)	Teflon/Pyrex with Borosilicate	Teflon/Pyrex with Borosilicate	Stainless steel	Teflon/Pyrex with Borosilicate	N/A
Residence time for reactive gases NO/NO <sub>2</sub> /NO <sub>y</sub> , SO <sub>2</sub> , O <sub>3</sub> ; PAMS: VOCs, Carbonyls (seconds)	5.19	5.19	5.0	3.38	N/A
For low volume PM instruments (flow rate < 200 liters/minute), is any PM instrument within 1 m of the hivol? If yes, please list distance (meters) and instrument(s).	N/A	N/A	N/A	N/A	N/A
For high volume PM instrument (flow rate > 200 liters/minute), is any PM instrument within 2m of the hivol? If yes, please list distance (meters) and instrument(s).	N/A	N/A	N/A	N/A	N/A
Frequency of flow rate verification for manual PM samplers, including Pb samplers (routine checks)	N/A	N/A	N/A	N/A	N/A
Frequency of flow rate verification for automated PM analyzers (routine checks)	N/A	N/A	N/A	N/A	N/A
Frequency of one-point QC check (gaseous)	Daily	Daily	N/A	Daily	N/A
Date of Annual Performance Evaluation conducted in the past calendar year for gaseous parameters (MM/DD/YYYY)	03/16/17	03/16/17	N/A	N/A	N/A
Date of two semi-annual flow rate audits conducted in the past calendar year for PM monitors (MM/DD/YYYY, MM/DD/YYYY)	N/A	N/A	N/A	N/A	N/A
Changes planned within the next 18 months (Y/N)	N	N	N	N	N

<b>Site Name</b>	<b>Fresno – Garland</b>
<b>AQS ID (XX-XXX-XXXX)</b>	06-019-0011
<b>Representative statistical area Name (i.e. MSA, CBSA, other)</b>	Fresno
<b>County</b>	Fresno
<b>Collecting (Operating) Agency</b>	CARB
<b>Analytical Lab (i.e. weigh lab, toxics lab, other)</b>	CARB
<b>Reporting Agency</b>	CARB
<b>Site Start Date</b>	12/31/2011
<b>Pollutant Parameters</b>	Ozone, PM10 STP FEM, PM2.5 FEM, PM2.5 FRM, PM2.5 Speciation (STN), CO, NO <sub>2</sub> , NO <sub>y</sub> , SO <sub>2</sub> , Lead, Toxics <b>PM<sub>10-2.5</sub></b> : (2) PM10 FEMs + (2) PM2.5 FEMs = (2) PM <sub>10-2.5</sub> FEMs. There are 2 pairs of analyzers - 1 pair is collocated. The (4) analyzers render (6) datasets. Each dataset has (3) method codes.
<b>Meteorological Parameters</b>	Wind speed, wind direction, outdoor temperature, barometric pressure, relative humidity
<b>Address</b>	3727 N. First St., Ste.104, Fresno CA 93726
<b>GPS Coordinates (decimal degrees)</b>	36.7853 N, -119.7732 W
<b>Distance to roadways (meters)</b>	30 m (south)
<b>Traffic Count/Year</b>	7,460/2011 (Raw traffic count in a 24-hour period: First Street near Dakota Avenue, Source: Fresno COG Fresno County Regional Traffic Monitoring Report 2013.)
<b>Groundcover (e.g. paved, vegetative, dirt, sand, gravel)</b>	Paved

Fresno–Garland (1)						
Pollutant	Ozone	CO	NO <sub>2</sub>	SO <sub>2</sub>	NOy	Toxics
Parameter code	44201	42101	42602	42401	42600	Many
Spatial scale	U	U	U	U	U	N
Site type	PE	PE	Max PEI	PE	PE	PE
Basic monitoring objective(s)	NC, RS	NC, RS	NC, RS	NC, RS	NC, RS	RS, TP
Monitor type	SLAMS	SLAMS	SLAMS	SLAMS	SLAMS	SLAMS
Network affiliation	NCore	NCore	NCore	NCore	NCore	NCore
FRM/FEM/ARM/Other	FEM	FRM	FRM	FEM	Other	Other
POC	1	3	1	1	3	Many
Primary / QA Collocated / Other (provide for all PM <sub>2.5</sub> , PM <sub>10</sub> , PM <sub>10-2.5</sub> , Pb and NO <sub>2</sub> monitors. Non-PM, Pb, NO <sub>2</sub> monitors should be listed as "N/A".)	N/A	N/A	N/A	N/A	Primary	Other
Is it suitable for comparison against the annual PM <sub>2.5</sub> ? (Y/N)	N/A	N/A	N/A	N/A	N/A	N/A
Instrument manufacturer and model	Teledyne API 400	API 300 EU	API 200E	Thermo 43	Instrumental	Xontech 924
Analysis method	UV	UV	UV	UV	Chem. Teledyne API 200EU/501	Many
Method code	087	093	099	009	699	Many
Monitoring start date (MM/DD/YYYY)	12/23/2011	01/18/2012	02/1/2012	01/18/2012	01/18/2012	12/23/2011
Required sampling frequency (e.g. 1:3 excluding exceptional events/1:1 including exceptional events)	Hourly	Hourly	Hourly	Hourly	Hourly	Hourly
Sampling season (MM/DD - MM/DD)	01/01 – 12/31	01/01 – 12/31	01/01 – 12/31	01/01 – 12/31	01/01 – 12/31	01/01 – 12/31
Probe/Inlet height above ground (meters)	7.0 m	7.0 m	7.0 m	7.0 m	6.2 m	5.8 m
Distance from supporting structure (meters)	N/A	N/A	N/A	N/A	N/A	N/A
Distance from obstructions on roof. Include horizontal distance + vertical height above probe for obstructions nearby. (meters)	N/A	N/A	N/A	N/A	N/A	N/A



Pollutant	Ozone	CO	NO2	SO2	NOy	Toxics
Distance from obstructions not on roof. Include horizontal distance + vertical height above probe for obstructions nearby. (meters)	N/A	N/A	N/A	N/A	N/A	N/A
Distance from trees (meters)	N/A	N/A	N/A	N/A	N/A	N/A
Distance to furnace or incinerator flue (meters)	N/A	N/A	N/A	N/A	N/A	N/A
Distance between collocated monitors (meters)	N/A	N/A	N/A	N/A	N/A	N/A
Unrestricted airflow (degrees)	360	360	360	360	360	360
Probe material (Teflon, etc.)	Teflon	Teflon	Teflon	Teflon	Teflon	Teflon
Residence time (seconds)	7.5	7.1	6.7	7.2	< 20 seconds	
For low volume PM instruments (flow rate < 200 liters/minute), is any PM instrument within 1 m of the hivol? If yes, please list distance (meters) and instrument(s).	N/A	N/A	N/A	N/A	N/A	N/A
For high volume PM instrument (flow rate > 200 liters/minute), is any PM instrument within 2m of the hivol? If yes, please list distance (meters) and instrument(s).	N/A	N/A	N/A	N/A	N/A	N/A
Frequency of flow rate verification for automated PM analyzers audit	N/A	N/A	N/A	N/A	N/A	N/A
Frequency of one-point QC check (gaseous)	Nightly	Nightly	Nightly	Nightly	Nightly	N/A
Last Annual Performance Evaluation (gaseous)	3/15/17	12/5/17	3/15/17	12/5/17	N/A	3/15/17
Last two semi-annual flow rate audits for PM monitors	N/A	N/A	N/A	N/A	N/A	N/A
Changes planned within the next 18 months (Y/N)	N	N	N	N	Y	N

Fresno–Garland (2)					
Pollutant	PM2.5	PM2.5	PM10 STP / PM10 LC	PM2.5	PM10-2.5
Parameter code	88101	88101	81102 / 85101	88101	86101
Spatial scale	N	N	N	N	N
Site type	HC	HC, PE, QA	PE	HC, QA	PE, QA
Basic monitoring objective(s)	NC, RS	NC, RS	NC, RS	NC, RS	NC, RS
Monitor type	SLAMS	SLAMS	SLAMS	SLAMS	SLAMS
Network affiliation	NCore	NCore	NCore	NCore	NCore
FRM/FEM/ARM/Other	FRM	FRM	FEM	FEM	FEM
POC	1	2	3 / 4	3 / 4	3 / 4
Primary / QA Collocated / Other (provide for all PM <sub>2.5</sub> , PM <sub>10</sub> , PM <sub>10-2.5</sub> , Pb and NO <sub>2</sub> monitors. Non-PM, Pb, NO <sub>2</sub> monitors should be listed as "N/A".)	Primary	QA Collocated	Primary	QA Collocated	QA Collocated, serving as Primary
Is it suitable for comparison against the annual PM <sub>2.5</sub> ? (Y/N)	Y	Y	N/A	Y	N/A
Instrument manufacturer and model	R&P 2025	R&P 2025	Met One BAM 1020 (QTY 2)	MetOne BAM 1020 (QTY 2)	Met One BAM 1020 (QTY 2)
Analysis method	Sequential	Sequential	Beta Attenuation	Beta Attenuation	Beta Attenuation
Method code	145	145	122	170	185
Monitoring start date (MM/DD/YYYY)	1/1/2012	1/25/2012	1/1/2012	1/1/2012	10/14/2013
Required sampling frequency (e.g. 1:3 excluding exceptional events/1:1 including exceptional events)	1:1	1:6	Hourly	Hourly	Hourly
Sampling season (MM/DD - MM/DD)	01/01 – 12/31	01/01 – 12/31	01/01 – 12/31	01/01 – 12/31	01/01 – 12/31
Probe/Inlet height above ground (meters)	5.9 m	5.9 m	6.2 m	6.4 m	6.3 m
Distance from supporting structure (meters)	N/A	N/A	N/A	N/A	N/A
Distance from obstructions on roof. Include horizontal distance + vertical height above probe for obstructions nearby. (meters)	N/A	N/A	N/A	N/A	N/A
Distance from obstructions not on roof. Include horizontal distance + vertical height above probe for obstructions nearby. (meters)	N/A	N/A	N/A	N/A	N/A
Distance from trees (meters)	N/A	N/A	N/A	N/A	N/A

Pollutant	PM2.5	PM2.5	PM10 STP	PM2.5	PM10-2.5
Distance to furnace or incinerator flue (meters)	N/A	N/A	N/A	N/A	N/A
Distance between collocated monitors (meters)	2.0 m	2.0 m	1.0 m	N/A	N/A
Unrestricted airflow (degrees)	360	360	360	360	360
Probe material (Teflon, etc.)	N/A	N/A	Aluminum	N/A	N/A
Residence time (seconds)	N/A	N/A	N/A	N/A	N/A
For low volume PM instruments (flow rate < 200 liters/minute), is any PM instrument within 1 m of the hivol? If yes, please list distance (meters) and instrument(s).	No	No	No	No	No
For high volume PM instrument (flow rate > 200 liters/minute), is any PM instrument within 2m of the hivol? If yes, please list distance (meters) and instrument(s).	N/A	N/A	N/A	N/A	N/A
Frequency of flow rate verification for manual PM samplers audit	Monthly	Monthly	Bi-weekly	Bi-weekly	Bi-weekly
Frequency of flow rate verification for automated PM analyzers audit	Monthly	Monthly	BI-weekly	BI-weekly	Bi-weekly
Frequency of one-point QC check (gaseous)	N/A	N/A	N/A	N/A	N/A
Last Annual Performance Evaluation (gaseous)	N/A	N/A	N/A	N/A	N/A
Last two semi-annual flow rate audits for PM monitors	03/15/2017, 09/18/2017	03/15/2017, 09/18/2017	03/15/2017, 09/18/2017	03/15/2017, 09/18/2017	03/15/2017, 09/18/2017
Changes planned within the next 18 months (Y/N)	N	N	Y	Y	Y

Fresno–Garland (3)					
Pollutant	Lead TSP (LC)	Lead TSP (STP)	PM2.5 Speciation	PM2.5 Speciation	Meteorology
Parameter code	14129	12128	Many	Many	61103, 61104, 62101, 62102, 62201
Spatial scale	N	N	N, U	N, U	U
Site type	PE	PE	PE	PE	GB
Monitor objective	NC, RS, TP	NC	RS	RS	RS, TP
Monitor type	SLAMS	SLAMS	Other	Other	SLAMS
Network affiliation	NCore	NCore	NCore, STN	NCore, STN	NCore
FRM/FEM/ARM/Other	FEM	Other	Other	Other	Other
POC	1	7	5	5	Many
Primary / QA Collocated / Other (provide for all PM <sub>2.5</sub> , PM <sub>10</sub> , PM <sub>10-2.5</sub> , Pb and NO <sub>2</sub> monitors. Non-PM, Pb, NO <sub>2</sub> monitors should be listed as "N/A".)	Primary	Primary	Primary	Primary	Other
Is it suitable for comparison against the annual PM <sub>2.5</sub> ? (Y/N)	N/A	N/A	N/A	N/A	N/A
Instrument manufacturer and model)	Hi-Vol	Lo-Vol Xontech 924, Teflon	Met-One SASS	URG 3000-N	RM Young 81000, Vaisala HMP 155
Method code	193	305	810	839	066, 059
Analysis method	ICP-MS	ICP/Mass Spectrometer	Many	Many	Many
Monitoring start date (MM/DD/YYYY)	2/1/2012	1/1/2012	1/1/2012	1/1/2012	12/23/2011
Required sampling frequency (e.g. 1:3 excluding exceptional events/1:1 including exceptional events)	1:6	1:6	1:3	1:3	Hourly
Sampling season (MM/DD - MM/DD)	01/01 – 12/31	01/01 – 12/31	01/01 – 12/31	01/01 – 12/31	01/01 – 12/31
Probe height (meters)	1.35 m	5.9 m	5.5 m	5.5 m	10 m
Distance from supporting structure (meters)	1.2 m	2.1 m	2 m	2 m	8 m
Distance from obstructions on roof. Include horizontal distance + vertical height above probe for obstructions nearby. (meters)	N/A	N/A	10 m	10 m	N/A
Distance from obstructions not on roof. Include horizontal distance + vertical height above probe for obstructions nearby. (meters)	N/A	N/A	11 m	9 m	N/A

Pollutant	Lead TSP (LC)	Lead TSP (STP)	PM2.5 Speciation	PM2.5 Speciation	Meteorology
Distance from trees (meters)	N/A	N/A	11 m	9 m	N/A
Distance to furnace or incinerator flue (meters)	2.4 m	2.4 m	9 m	9 m	N/A
Distance between collocated monitors (meters)	N/A	N/A	2.5 m	2.5 m	N/A
Unrestricted airflow (degrees)	360	360	360	360	360
Probe material (Teflon, etc.)	N/A	Teflon	N/A	N/A	Teflon
Residence time (seconds)	N/A	N/A	N/A	N/A	N/A
For low volume PM instruments (flow rate < 200 liters/minute), is any PM instrument within 1 m of the hivol? If yes, please list distance (meters) and instrument(s).	N/A	N/A	No	No	N/A
For high volume PM instrument (flow rate > 200 liters/minute), is any PM instrument within 2m of the hivol? If yes, please list distance (meters) and instrument(s).	No	No	N/A	N/A	N/A
Frequency of flow rate verification for manual PM samplers audit	Monthly	Monthly	Bi-weekly	Bi-weekly	N/A
Frequency of flow rate verification for automated PM analyzers audit	Monthly	Monthly	N/A	N/A	N/A
Frequency of one-point QC check (gaseous)	N/A	N/A	N/A	N/A	N/A
Last Annual Performance Evaluation (gaseous)	N/A	N/A	N/A	N/A	N/A
Last two semi-annual flow rate audits for PM monitors	03/15/2017, 09/18/2017	03/15/2017, 09/18/2017	9/18/2017	N/A	N/A
Changes planned within the next 18 months (Y/N)	N	Y	N	N	N

<b>Site Name</b>	<b>Fresno - Pacific</b>
<b>AQS ID (XX-XXX-XXXX)</b>	06-019-5025
<b>Representative statistical area Name (i.e. MSA, CBSA, other)</b>	Fresno
<b>County</b>	Fresno
<b>Collecting (Operating) Agency</b>	SJVAPCD
<b>Analytical Lab (i.e. weigh lab, toxics lab, other)</b>	CARB
<b>Reporting Agency</b>	CARB
<b>Site Start Date</b>	01/01/2000
<b>Pollutant Parameters</b>	PM2.5 FRM
<b>Meteorological Parameters</b>	None
<b>Address</b>	1716 Winery, Fresno, CA 93727
<b>GPS Coordinates (decimal degrees)</b>	36.7263N, -119.7330W
<b>Distance to roadways (meters)</b>	40 m (east)
<b>Traffic Count/Year</b>	8,540 / 2018 (Raw traffic count in a 24-hour period: Butler Avenue/Winery Avenue intersection, Source: Fresno COG Traffic Counts, 2007-2018 Kittelson & Associates, Inc.)
<b>Groundcover (e.g. paved, vegetative, dirt, sand, gravel)</b>	Vegetative and paved

Fresno – Pacific (1)	
<b>Pollutant</b>	<b>PM2.5</b>
Parameter code	88101
Spatial scale	N
Site type	PE
Basic monitoring objective(s)	NC, RS
Monitor type	SLAMS
Network affiliation(s), if applicable (a monitor may have none, one, or multiple)	None
FRM/FEM/ARM/Other	FRM
POC	1
Primary / QA Collocated / Other (provide for all PM <sub>2.5</sub> , PM <sub>10</sub> , PM <sub>10-2.5</sub> , Pb and NO <sub>2</sub> monitors. Non-PM, Pb, NO <sub>2</sub> monitors should be listed as "N/A".)	Primary
Is it suitable for comparison against the annual PM <sub>2.5</sub> ? (Y/N)	Y
Instrument manufacturer and model	Partisol 2025I
Analysis method	Gravimetric
Method code	145
Monitoring start date (MM/DD/YYYY)	01/01/2000
Required sampling frequency (e.g. 1:3 excluding exceptional events/1:1 including exceptional events)	1:3
Sampling season (MM/DD - MM/DD)	01/01 – 12/31
Probe height (meters)	11.3 m
Distance from supporting structure (meters)	2.1 m
Distance from obstructions on roof. Include horizontal distance + vertical height above probe for obstructions nearby. (meters)	None
Distance from obstructions not on roof. Include horizontal distance + vertical height above probe for obstructions nearby. (meters)	53.4m NE 5.1 above vertical
Distance from trees (meters)	77 m
Distance to furnace or incinerator flue (meters)	None
Distance between monitors fulfilling a QA collocation requirement (meters).	N/A

Pollutant	PM2.5
Unrestricted airflow (degrees around probe/inlet or percentage of monitoring path)	360
Probe material for reactive gases NO/NO <sub>2</sub> /NO <sub>y</sub> , SO <sub>2</sub> , O <sub>3</sub> ; PAMS: VOCs, Carbonyls (e.g. Pyrex, stainless steel, Teflon)	Aluminum
Residence time for reactive gases NO/NO <sub>2</sub> /NO <sub>y</sub> , SO <sub>2</sub> , O <sub>3</sub> ; PAMS: VOCs, Carbonyls (seconds)	N/A
For low volume PM instruments (flow rate < 200 liters/minute), is any PM instrument within 1 m of the hivol? If yes, please list distance (meters) and instrument(s).	No
For high volume PM instrument (flow rate > 200 liters/minute), is any PM instrument within 2m of the hivol? If yes, please list distance (meters) and instrument(s).	N/A
Frequency of flow rate verification for manual PM samplers, including Pb samplers (routine checks)	Biweekly
Frequency of flow rate verification for automated PM analyzers (routine checks)	N/A
Frequency of one-point QC check for gaseous instruments	N/A
Date of Annual Performance Evaluation conducted in the past calendar year for gaseous parameters (MM/DD/YYYY)	N/A
Date of two semi-annual flow rate audits conducted in the past calendar year for PM monitors (MM/DD/YYYY, MM/DD/YYYY)	03/01/17, 09/19/17
Changes planned within the next 18 months (Y/N)	N



<b>Site Name</b>	<b>Fresno - Drummond</b>	
<b>AQS ID (XX-XXX-XXXX)</b>	06-019-0007	
<b>Representative statistical area Name (i.e. MSA, CBSA, other)</b>	Fresno	
<b>County</b>	Fresno	
<b>Collecting (Operating) Agency</b>	SJVAPCD	
<b>Analytical Lab (i.e. weigh lab, toxics lab, other)</b>	CARB	
<b>Reporting Agency</b>	SJVAPCD: Ozone, NO2, PM2.5	CARB: PM10 FRM
<b>Site Start Date</b>	07/01/1984	
<b>Pollutant Parameters</b>	Ozone, PM10 FRM, NO2	
<b>Meteorological Parameters</b>	Wind speed, wind direction, outdoor temperature, barometric pressure	
<b>Address</b>	4706 E. Drummond Street, Fresno, CA 93725	
<b>GPS Coordinates (decimal degrees)</b>	36.7055 N, -119.7410 W	
<b>Distance to roadways (meters)</b>	50m	
<b>Traffic Count/Year</b>	27,251/2018 (Raw traffic count in a 24-hour period for nearest roads: Jensen Avenue between Chestnut Avenue and Maple Avenue, Source: Fresno COG Traffic Counts, 2007-2018 Kittelson & Associates, Inc.	
<b>Groundcover (e.g. paved, vegetative, dirt, sand, gravel)</b>	Paved	

Fresno – Drummond (1)					
Pollutant	Ozone	PM10	PM10	NO <sub>2</sub>	Meteorology
Parameter code	44201	81102	81102	42602	Many
Spatial scale	N	N	N	N	R
Site type	PE, HC, RT	PE	PE, QA	HC	GB
Basic monitoring objective(s)	NC, RS, TP	NC, RS	NC, RS	NC	RS, TP
Monitor type	SLAMS	SLAMS	SLAMS	SLAMS	Other
Network affiliation(s), if applicable (a monitor may have none, one, or multiple)	None	None	None	None	None
FRM/FEM/ARM/Other	FRM	FRM	FRM	FEM	Other
POC	1	1	2	1	1
Primary / QA Collocated / Other (provide for all PM <sub>2.5</sub> , PM <sub>10</sub> , PM <sub>10-2.5</sub> , Pb and NO <sub>2</sub> monitors. Non-PM, Pb, NO <sub>2</sub> monitors should be listed as “N/A”.)	Primary	Primary	QA Collocated	N/A	Other
Is it suitable for comparison against the annual PM <sub>2.5</sub> ? (Y/N)	N/A	N/A	N/A	N/A	N/A
Instrument manufacturer and model	Teledyne API T265	ECOTECH Hi-Vol 3000	ECOTECH Hi-Vol 3000	Teledyne API T200	ITP- HY-CAL BAAA3B, OT-Met One 060A-2, BP- Met One 092, WD- Met One 020C, WS-Met One 010C
Analysis method	Chem.	Gravimetric	Gravimetric	CL	Many
Method code	199	162	162	099	Many
Monitoring start date (MM/DD/YYYY)	05/01/2017	07/01/1984	07/01/1984	03/01/2017	07/01/1984
Required sampling frequency (e.g. 1:3 excluding exceptional events/1:1 including exceptional events)	Hourly	1:6	1:6	Hourly	Hourly
Sampling season (MM/DD - MM/DD)	01/01 – 12/31	01/01 – 12/31	01/01 – 12/31	01/01 - 12/31	01/01 – 12/31
Probe height (meters)	8.0 m	5.23 m	5.23 m	8.0 m	9.8 m
Distance from supporting structure (meters)	4.37 m	1.58 m	1.58 m	4.37 m	N/A
Distance from obstructions on roof. Include horizontal distance + vertical height above probe for obstructions nearby. (meters)	N/A	N/A	N/A	N/A	N/A
Distance from obstructions not on roof. Include horizontal distance + vertical height above probe for obstructions nearby. (meters)	N/A	7.0 mH, 0.76 mV	3.35 mH, 0.76 mV	N/A	N/A

Pollutant	Ozone	PM10	PM10	NO <sub>2</sub>	Meteorology
Distance from trees (meters)	15.3 m	15.3 m	18.8 m	15.3 m	17.2 m
Distance to furnace or incinerator flue (meters)	N/A	N/A	N/A	N/A	N/A
Distance between monitors fulfilling a QA collocation requirement (meters).	N/A	3.9 m	3.9 m	N/A	N/A
Unrestricted airflow (degrees around probe/inlet or percentage of monitoring path)	360	340	340	360	360
Probe material for reactive gases NO/NO <sub>2</sub> /NO <sub>y</sub> , SO <sub>2</sub> , O <sub>3</sub> ; PAMS: VOCs, Carbonyls (e.g. Pyrex, stainless steel, Teflon)	Teflon/Pyrex with Borosilicate	N/A	N/A	Teflon/Pyrex with Borosilicate	N/A
Residence time for reactive gases NO/NO <sub>2</sub> /NO <sub>y</sub> , SO <sub>2</sub> , O <sub>3</sub> ; PAMS: VOCs, Carbonyls (seconds)	8.7	N/A	N/A	9.1	N/A
Frequency of one-point QC check for gaseous instruments	Daily	N/A	N/A	Daily	N/A
Frequency of flow rate verification for manual PM samplers, including Pb samplers (routine checks)	N/A	Monthly	Monthly	N/A	N/A
Frequency of flow rate verification for automated PM analyzers (routine checks)	N/A	None	None	N/A	N/A
For low volume PM instruments (flow rate < 200 liters/minute), is any PM instrument within 1 m of the hivol? If yes, please list distance (meters) and instrument(s).	N/A	None	None	N/A	N/A
For high volume PM instrument (flow rate > 200 liters/minute), is any PM instrument within 2m of the hivol? If yes, please list distance (meters) and instrument(s).	N/A	No	No	N/A	N/A
Date of Annual Performance Evaluation conducted in the past calendar year for gaseous parameters (MM/DD/YYYY)	2/22/18	N/A	N/A	02/22/18	N/A
Date of two semi-annual flow rate audits conducted in the past calendar year for PM monitors (MM/DD/YYYY, MM/DD/YYYY)	N/A	9/19/17, 2/22/18	9/19/17, 2/22/18	N/A	N/A
Changes planned within the next 18 months (Y/N)	N	N	N	N	N

<b>Site Name</b>	<b>Fresno - Foundry</b>
<b>AQS ID (XX-XXX-XXXX)</b>	06-019-2016
<b>Representative statistical area Name (i.e. MSA, CBSA, other)</b>	Fresno
<b>County</b>	Fresno
<b>Collecting (Operating) Agency</b>	SJVAPCD
<b>Analytical Lab (i.e. weigh lab, toxics lab, other)</b>	N/A
<b>Reporting Agency</b>	SJVAPCD
<b>Site Start Date</b>	01/01/2016
<b>Pollutant Parameters</b>	NO2
<b>Meteorological Parameters</b>	Wind speed, wind direction, outdoor temperature, barometric pressure
<b>Address</b>	2482 Foundry Park Ave, Fresno, CA 93706
<b>GPS Coordinates (decimal degrees)</b>	36.710833N, -119.7775W
<b>Distance to roadways (meters)</b>	16 to 19 meters
<b>Traffic Count/Year</b>	114,000/2016 (Rte 99 and Jensen Avenue off-ramp, Source: Caltrans 2016 )
<b>Groundcover (e.g. paved, vegetative, dirt, sand, gravel)</b>	Paved

<b>Fresno – Foundry (1)</b>		
<b>Pollutant</b>	<b>NO<sub>2</sub></b>	<b>Meteorology</b>
Parameter code	42602	Many
Spatial scale	MC	N
Site type	HC	PE
Basic monitoring objective(s)	NC, RS, TP	RS, TP
Monitor type	SLAMS	Other
Network affiliation(s), if applicable (a monitor may have none, one, or multiple)	Near-road	Near-road
FRM/FEM/ARM/Other	FEM	Other
POC	1	Many
Primary / QA Collocated / Other (provide for all PM <sub>2.5</sub> , PM <sub>10</sub> , PM <sub>10-2.5</sub> , Pb and NO <sub>2</sub> monitors. Non-PM, Pb, NO <sub>2</sub> monitors should be listed as “N/A”.)	Primary	Other
Is it suitable for comparison against the annual PM <sub>2.5</sub> ? (Y/N)	N/A	N/A
Instrument manufacturer and model	Teledyne T500U	ITP – Hamp. Control 140-100Hv, OT – MET One 060-A-2, BP – MET One 092, WD – MET One 020C, WS – METOne 010C
Analysis method	CL	Many
Method code	212	Many
Monitoring start date (MM/DD/YYYY)	01/01/2016	01/01/2016
Required sampling frequency (e.g. 1:3 excluding exceptional events/1:1 including exceptional events)	Hourly	Hourly
Sampling season (MM/DD - MM/DD)	01/01 – 12/31	01/01 – 12/31
Probe height (meters)	5.7 m	5.9 m
Distance from supporting structure (meters)	1.8 m	2.0 m
Distance from obstructions on roof. Include horizontal distance + vertical height above probe for obstructions nearby. (meters)	N/A	N/A
Distance from obstructions not on roof. Include horizontal distance + vertical height above probe for obstructions nearby. (meters)	26.3m H (north), 4m V 37m H (east), 4m V	26.3m H (north), 4m V 37m H (east), 4m V
Distance from trees (meters)	8.45 m	8.5 m
Distance to furnace or incinerator flue (meters)	N/A	N/A

Pollutant	NO <sub>2</sub>	Meteorology
Distance between monitors fulfilling a QA collocation requirement (meters).	N/A	N/A
Unrestricted airflow (degrees around probe/inlet or percentage of monitoring path)	350	350
Probe material for reactive gases NO/NO <sub>2</sub> /NO <sub>y</sub> , SO <sub>2</sub> , O <sub>3</sub> ; PAMS: VOCs, Carbonyls (e.g. Pyrex, stainless steel, Teflon)	Teflon/Pyrex with Borosilicate	N/A
Residence time for reactive gases NO/NO <sub>2</sub> /NO <sub>y</sub> , SO <sub>2</sub> , O <sub>3</sub> ; PAMS: VOCs, Carbonyls (seconds)	3.20	N/A
Frequency of one-point QC check for gaseous instruments	Daily	N/A
Frequency of flow rate verification for manual PM samplers, including Pb samplers (routine checks)	N/A	N/A
Frequency of flow rate verification for automated PM analyzers (routine checks)	N/A	N/A
For low volume PM instruments (flow rate < 200 liters/minute), is any PM instrument within 1 m of the hivol? If yes, please list distance (meters) and instrument(s).	N/A	N/A
For high volume PM instrument (flow rate > 200 liters/minute), is any PM instrument within 2m of the hivol? If yes, please list distance (meters) and instrument(s).	N/A	N/A
Date of Annual Performance Evaluation conducted in the past calendar year for gaseous parameters (MM/DD/YYYY)	N/A	N/A
Date of two semi-annual flow rate audits conducted in the past calendar year for PM monitors (MM/DD/YYYY, MM/DD/YYYY)	N/A	N/A
Changes planned within the next 18 months (Y/N)	N	N

<b>Site Name</b>	<b>Parlier</b>
<b>AQS ID (XX-XXX-XXXX)</b>	06-019-4001
<b>Representative statistical area Name (i.e. MSA, CBSA, other)</b>	Fresno
<b>County</b>	Fresno
<b>Collecting (Operating) Agency</b>	SJVAPCD
<b>Analytical Lab (i.e. weigh lab, toxics lab, other)</b>	Varies based on which laboratory is contracted with the SJVAPCD: Speciated VOC
<b>Reporting Agency</b>	SJVAPCD
<b>Site Start Date</b>	6/1/1983
<b>Pollutant Parameters</b>	Ozone, NO2, Speciated VOC, NMH
<b>Meteorological Parameters</b>	Wind speed, wind direction, outdoor temperature, relative humidity, barometric pressure, solar radiation
<b>Address</b>	9240 S. Riverbend Ave., Parlier, CA 93648
<b>GPS Coordinates (decimal degrees)</b>	36.5972 N, -119.5040 W
<b>Distance to roadways (meters)</b>	100 m (east)
<b>Traffic Count/Year</b>	21,260/2018 (Raw traffic count in a 24-hour period for nearest roads: E. Manning Avenue between S. Mendocino Avenue and S. Newmark Avenue, Source: Fresno COG Traffic Counts, 2007-2018 Kittelson & Associates, Inc.)
<b>Groundcover (e.g. paved, vegetative, dirt, sand, gravel)</b>	Dirt, vegetation

Parlier (1)					
Pollutant	Ozone	NO <sub>2</sub>	Speciated VOC	NMH	Meteorology
Parameter code	44201	42602	Many	43102	Many
Spatial scale	N	N	N	N	R
Site type	HC, RT	PE	PE	PE	GB
Basic monitoring objective(s)	NC, RS, TP	NC, RS, TP	RS	RS, TP	RS, TP
Monitor type	SLAMS	SLAMS	Other	Other	Many
Network affiliation(s), if applicable (a monitor may have none, one, or multiple)	PAMS	PAMS, RA40	PAMS	PAMS	PAMS
FRM/FEM/ARM/Other	FEM	FEM	Other	Other	Other
POC	1	1	1	1	1
Primary / QA Collocated / Other (provide for all PM <sub>2.5</sub> , PM <sub>10</sub> , PM <sub>10-2.5</sub> , Pb and NO <sub>2</sub> monitors. Non-PM, Pb, NO <sub>2</sub> monitors should be listed as "N/A".)	N/A	N/A	N/A	N/A	Other
Is it suitable for comparison against the annual PM <sub>2.5</sub> ? (Y/N)	N/A	N/A	N/A	N/A	N/A
Instrument manufacturer and model	Teledyne 400E	Teledyne 200E	Xontech 910A	Synspec 115	ITP- Hy-Cal 512AA3B, OT- Met One 060A-2, BP- Met One 092, RH- Vaisala HMP45D, SRD-Epplly Mod.8-48, WD- Met One 020C, WS- Met One 010C
Analysis method	UV	CL	GC	GC	Many
Method code	087	099	126	011	Many
Monitoring start date (MM/DD/YYYY)	06/01/1983	06/01/1983	06/01/1983	06/01/1983	06/01/1983
Required sampling frequency (e.g. 1:3 excluding exceptional events/1:1 including exceptional events)	Hourly	Hourly	1:3	Hourly	Hourly
Sampling season (MM/DD - MM/DD)	01/01 – 12/31	01/01 – 12/31	06/01 – 08/31	01/01 – 12/31	01/01 - 12/31
Probe height (meters)	8.7 m	8.7 m	8.7 m	8.7 m	9.1 m
Distance from supporting structure (meters)	2.7 m	2.7m	2.7 m	2.7 m	4.9 m



Pollutant	Ozone	NO <sub>2</sub>	Speciated VOC	NMH	Meteorology
Distance from obstructions on roof. Include horizontal distance + vertical height above probe for obstructions nearby. (meters)	None	None	None	None	None
Distance from obstructions not on roof. Include horizontal distance + vertical height above probe for obstructions nearby. (meters)	39.0 m	39.0 m	39.0 m	39.0 m	38.9 m
Distance from trees (meters)	11.0 m	11.0 m	11.0 m	11.0 m	10.2 m
Distance to furnace or incinerator flue (meters)	N/A	N/A	N/A	N/A	N/A
Distance between monitors fulfilling a QA collocation requirement (meters).	N/A	N/A	N/A	N/A	N/A
Unrestricted airflow (degrees around probe/inlet or percentage of monitoring path)	360	360	360	360	360
Probe material for reactive gases NO/NO <sub>2</sub> /NO <sub>y</sub> , SO <sub>2</sub> , O <sub>3</sub> ; PAMS: VOCs, Carbonyls (e.g. Pyrex, stainless steel, Teflon)	Teflon/Pyrex with Borosilicate	Teflon/Pyrex with Borosilicate	Stainless steel	Teflon/Pyrex with Borosilicate	N/A
Residence time for reactive gases NO/NO <sub>2</sub> /NO <sub>y</sub> , SO <sub>2</sub> , O <sub>3</sub> ; PAMS: VOCs, Carbonyls (seconds)	10.3	9.98	4.69	13.97	N/A
Frequency of one-point QC check for gaseous instruments	daily	daily	daily	daily	N/A
Frequency of flow rate verification for manual PM samplers, including Pb samplers (routine checks)	N/A	N/A	N/A	N/A	N/A
Frequency of flow rate verification for automated PM analyzers (routine checks)	N/A	N/A	N/A	N/A	N/A

Pollutant	Ozone	NO <sub>2</sub>	Speciated VOC	NMH	Meteorology
For low volume PM instruments (flow rate < 200 liters/minute), is any PM instrument within 1 m of the lovol? If yes, please list distance (meters) and instrument(s).	N/A	N/A	N/A	N/A	N/A
For high volume PM instrument (flow rate > 200 liters/minute), is any PM instrument within 2m of the hivol? If yes, please list distance (meters) and instrument(s).	N/A	N/A	N/A	N/A	N/A
Date of Annual Performance Evaluation conducted in the past calendar year for gaseous parameters (MM/DD/YYYY)	12/14/17	12/14/17	N/A	N/A	N/A
Date of two semi-annual flow rate audits conducted in the past calendar year for PM monitors (MM/DD/YYYY, MM/DD/YYYY)	N/A	N/A	N/A	N/A	N/A
Changes planned within the next 18 months (Y/N)	N	N	N	N	N

<b>Site Name</b>	<b>Huron</b>
<b>AQS ID (XX-XXX-XXXX)</b>	06-019-2008
<b>Representative statistical area Name (i.e. MSA, CBSA, other)</b>	Fresno
<b>County</b>	Fresno
<b>Collecting (Operating) Agency</b>	SJVAPCD
<b>Analytical Lab (i.e. weigh lab, toxics lab, other)</b>	N/A
<b>Reporting Agency</b>	SJVAPCD
<b>Site Start Date</b>	09/01/09
<b>Pollutant Parameters</b>	PM2.5 Non-FEM
<b>Meteorological Parameters</b>	Barometric Pressure
<b>Address</b>	16875 4 <sup>th</sup> St, Huron, CA 93234
<b>GPS Coordinates (decimal degrees)</b>	36.2363 N, -119.7656 W
<b>Distance to roadways (meters)</b>	100 m (north)
<b>Traffic Count/Year</b>	3,450/2016 (Traffic count for nearest roads: Rte 269/Rte 198, Source: Caltrans 2016)
<b>Groundcover (e.g. paved, vegetative, dirt, sand, gravel)</b>	Paved, vegetative

<b>Huron (1)</b>		
<b>Pollutant</b>	<b>PM2.5</b>	<b>Meteorology</b>
Parameter code	88502	64101
Spatial scale	N	N
Site type	PE	PE
Basic monitoring objective(s)	TP	TP
Monitor type	SPM	Other
Network affiliation(s), if applicable (a monitor may have none, one, or multiple)	None	None
FRM/FEM/ARM/Other	Non-FEM	Other
POC	3	1
Primary / QA Collocated / Other (provide for all PM <sub>2.5</sub> , PM <sub>10</sub> , PM <sub>10-2.5</sub> , Pb and NO <sub>2</sub> monitors. Non-PM, Pb, NO <sub>2</sub> monitors should be listed as "N/A".)	N/A	N/A
Is it suitable for comparison against the annual PM <sub>2.5</sub> ? (Y/N)	N	N/A
Instrument manufacturer and model	MET One BAM 1020	ITP – Hy-Cal BA-512-A-A-3-B, BP – Met One 092
Analysis method	Beta-Attenuation	Many
Method code	731	014
Monitoring start date (MM/DD/YYYY)	09/12/2009	02/01/2010
Required sampling frequency (e.g. 1:3 excluding exceptional events/1:1 including exceptional events)	Hourly	Hourly
Sampling season (MM/DD - MM/DD)	01/01 – 12/31	01/01 – 12/31
Probe height (meters)	6.42 m	10 m
Distance from supporting structure (meters)	1.14 m	N/A
Distance from obstructions on roof. Include horizontal distance + vertical height above probe for obstructions nearby. (meters)	N/A	N/A
Distance from obstructions not on roof. Include horizontal distance + vertical height above probe for obstructions nearby. (meters)	N/A	N/A
Distance from trees (meters)	41.5 m	N/A
Distance to furnace or incinerator flue (meters)	N/A	N/A
Distance between monitors fulfilling a QA collocation requirement (meters).	N/A	N/A
Unrestricted airflow (degrees around probe/inlet or percentage of monitoring path)	360	360

Pollutant	PM2.5	Meteorology
Probe material for reactive gases NO/NO <sub>2</sub> /NO <sub>y</sub> , SO <sub>2</sub> , O <sub>3</sub> ; PAMS: VOCs, Carbonyls (e.g. Pyrex, stainless steel, Teflon)	N/A	N/A
Residence time for reactive gases NO/NO <sub>2</sub> /NO <sub>y</sub> , SO <sub>2</sub> , O <sub>3</sub> ; PAMS: VOCs, Carbonyls (seconds)	N/A	N/A
Frequency of one-point QC check for gaseous instruments	N/A	N/A
Frequency of flow rate verification for manual PM samplers, including Pb samplers (routine checks)	N/A	N/A
Frequency of flow rate verification for automated PM analyzers (routine checks)	Bi-Weekly	N/A
For low volume PM instruments (flow rate < 200 liters/minute), is any PM instrument within 1 m of the hivol? If yes, please list distance (meters) and instrument(s).	None	N/A
For high volume PM instrument (flow rate > 200 liters/minute), is any PM instrument within 2m of the hivol? If yes, please list distance (meters) and instrument(s).	None	N/A
Date of Annual Performance Evaluation conducted in the past calendar year for gaseous parameters (MM/DD/YYYY)	N/A	N/A
Date of two semi-annual flow rate audits conducted in the past calendar year for PM monitors (MM/DD/YYYY, MM/DD/YYYY)	05/16/17, 11/15/17	N/A
Changes planned within the next 18 months (Y/N)	N	N

<b>Site Name</b>	<b>Hanford – Irwin</b>	
<b>AQS ID (XX-XXX-XXXX)</b>	06-031-1004	
<b>Representative statistical area Name (i.e. MSA, CBSA, other)</b>	Hanford-Corcoran	
<b>County</b>	Kings	
<b>Collecting (Operating) Agency</b>	SJVAPCD	
<b>Analytical Lab (i.e. weigh lab, toxics lab, other)</b>	CARB: PM10 FRM	
<b>Reporting Agency</b>	SJVAPCD: Ozone, PM10 FEM, PM2.5 FEM, NO2, Meteorology	CARB: PM10 FRM
<b>Site Start Date</b>	10/11/1993	
<b>Pollutant Parameters</b>	Ozone, PM10 FRM, PM10 FEM, PM2.5 FEM, NO2	
<b>Meteorological Parameters</b>	Wind speed, wind direction, outdoor temperature, barometric pressure	
<b>Address</b>	807 S. Irwin St., Hanford, CA 93230	
<b>GPS Coordinates (decimal degrees)</b>	36.3147 N, -119.6440 W	
<b>Distance to roadways (meters)</b>	60 m (east)	
<b>Traffic Count/Year</b>	9,647/2016 (Traffic count for nearest roads: Hanford-Armona Rd east of S. Williams St., Source: City of Hanford Public Works - Engineering, Traffic Counts Volume Summary 2017 – City of Hanford.)	
<b>Groundcover (e.g. paved, vegetative, dirt, sand, gravel)</b>	Paved, vegetative	

Hanford – Irwin (1)					
Pollutant	Ozone	PM2.5	PM2.5	NO <sub>2</sub>	Meteorology
Parameter code	44201	88101	88101	42602	Many
Spatial scale	N	N	N	N	N
Site type	HC, PE	PE	PE	PE	PE
Basic monitoring objective(s)	NC, RS, TP	NC, RS, TP	NC, RS, TP	NC, RS, TP	RS, TP
Monitor type	SLAMS	SLAMS	SLAMS	SLAMS	Many
Network affiliation(s), if applicable (a monitor may have none, one, or multiple)	None	None	None	None	None
FRM/FEM/ARM/Other	FEM	FEM	FEM	FEM	Other
POC	1	3	3	1	Many
Primary / QA Collocated / Other (provide for all PM <sub>2.5</sub> , PM <sub>10</sub> , PM <sub>10-2.5</sub> , Pb and NO <sub>2</sub> monitors. Non-PM, Pb, NO <sub>2</sub> monitors should be listed as "N/A".)	N/A	Other	Primary	N/A	Other
Is it suitable for comparison against the annual PM <sub>2.5</sub> ? (Y/N)	N/A	Y	Y	N/A	N/A
Instrument manufacturer and model	Teledyne 400E	MET One BAM 1020	Teledyne 602	Teledyne 200E	ITP- Hy-Cal 512AA3B, OT- Met One 060A-2, BP- Met One 092, WD- Met One 020C, WS-Met One 010C
Analysis method	UV	Beta Attenuation	Beta Attenuation	CL	Many
Method code	087	170	204	099	Many
Monitoring start date (MM/DD/YYYY)	02/25/2010	02/25/2010 End Date 10/31/17	11/01/2017	02/25/2010	02/25/2010
Required sampling frequency (e.g. 1:3 excluding exceptional events/1:1 including exceptional events)	Hourly	Hourly	Hourly	Hourly	Hourly
Sampling season (MM/DD - MM/DD)	01/01 – 12/31	01/01 – 12/31	01/01 – 12/31	01/01 – 12/31	01/01 – 12/31
Probe height (meters)	4.7 m	4.4 m	4.5 m	4.7 m	9.7 m
Distance from supporting structure (meters)	1.8 m	1.8 m	1.8 m	1.8 m	N/A

Pollutant	Ozone	PM2.5	PM2.5	NO <sub>2</sub>	Meteorology
Distance from obstructions on roof. Include horizontal distance + vertical height above probe for obstructions nearby. (meters)	N/A	N/A	N/A	N/A	N/A
Distance from obstructions not on roof. Include horizontal distance + vertical height above probe for obstructions nearby. (meters)	24.2 mV, 2.5 mH	26.5 mV, 2.5 mH	26.5 mV, 2.5 mH	24.2 mV, 2.5 mH	N/A
Distance from trees (meters)	26.5 m	29.5 m	29.5 m	26.5 m	26.6 m
Distance to furnace or incinerator flue (meters)	23.5 m	22.8 m	23.3 m	23.5 m	N/A
Distance between monitors fulfilling a QA collocation requirement (meters).	N/A	N/A	N/A	N/A	N/A
Unrestricted airflow (degrees around probe/inlet or percentage of monitoring path)	353.2	360	353.2	353.2	360
Probe material for reactive gases NO/NO <sub>2</sub> /NO <sub>y</sub> , SO <sub>2</sub> , O <sub>3</sub> ; PAMS: VOCs, Carbonyls (e.g. Pyrex, stainless steel, Teflon)	Teflon/Pyrex with Borosilicate	N/A	N/A	Teflon/Pyrex with Borosilicate	N/A
Residence time for reactive gases NO/NO <sub>2</sub> /NO <sub>y</sub> , SO <sub>2</sub> , O <sub>3</sub> ; PAMS: VOCs, Carbonyls (seconds)	12.8	N/A	N/A	13.1	N/A
Frequency of one-point QC check for gaseous instruments	Daily	N/A	N/A	Daily	N/A
Frequency of flow rate verification for manual PM samplers, including Pb samplers (routine checks)	N/A	N/A	N/A	N/A	N/A
Frequency of flow rate verification for automated PM analyzers (routine checks)	N/A	Biweekly	Biweekly	N/A	N/A
For low volume PM instruments (flow rate < 200 liters/minute), is any PM instrument within 1 m of the lovol? If yes, please list distance (meters) and instrument(s).	N/A	No	No	N/A	N/A



Pollutant	Ozone	PM2.5	PM2.5	NO <sub>2</sub>	Meteorology
For high volume PM instrument (flow rate > 200 liters/minute), is any PM instrument within 2m of the hivol? If yes, please list distance (meters) and instrument(s).	N/A	No	No	N/A	N/A
Date of Annual Performance Evaluation conducted in the past calendar year for gaseous parameters (MM/DD/YYYY)	10/24/17	N/A	N/A	10/24/17	N/A
Date of two semi-annual flow rate audits conducted in the past calendar year for PM monitors (MM/DD/YYYY, MM/DD/YYYY)	N/A	05/02/17, 10/24/17	10/24/17	N/A	N/A
Changes planned within the next 18 months (Y/N)	N	N	N	N	N

Hanford – Irwin (2)				
Pollutant	PM10 LC	PM10 STP	PM10 STP	PM10 STP / LC
Parameter code	85101	81102	81102	81102 / 85101
Spatial scale	N	N	N	N
Site type	PE	PE	PE	PE
Basic monitoring objective(s)	RS, TP	NC, RS, TP	NC, RS	NC, RS, TP / RS, TP
Monitor type	Other	SLAMS	SLAMS	SLAMS / Other
Network affiliation(s), if applicable (a monitor may have none, one, or multiple)	None	None	None	None
FRM/FEM/ARM/Other	FEM	FEM	FRM	FEM
POC	3	3	1	3 / 3
Primary / QA Collocated / Other (provide for all PM <sub>2.5</sub> , PM <sub>10</sub> , PM <sub>10-2.5</sub> , Pb and NO <sub>2</sub> monitors. Non-PM, Pb, NO <sub>2</sub> monitors should be listed as “N/A”.)	Other	Primary	Primary	Other
Is it suitable for comparison against the annual PM <sub>2.5</sub> ? (Y/N)	N	N	N/A	N/A
Instrument manufacturer and model	Teledyne 602	Teledyne 602	ECOTECH Hi-Vol 3000	Thermo TEOM 1400

Pollutant	PM10 LC	PM10 STP	PM10 STP	PM10 STP / LC
Analysis method	Beta Attenuation	Beta Attenuation	Gravimetric	Tapered Element
Method code	205	205	162	079
Monitoring start date (MM/DD/YYYY)	11/01/2017	11/01/2017	04/01/2015	Start Date: 07/14/2010 End Date: 10/31/17
Required sampling frequency (e.g. 1:3 excluding exceptional events/1:1 including exceptional events)	Hourly	Hourly	1:6	Hourly
Sampling season (MM/DD - MM/DD)	01/01 – 12/31	01/01 – 12/31	01/01 – 12/31	01/01 – 12/31
Probe height (meters)	4.6 m	4.8 m	4.5 m	4.4 m
Distance from supporting structure (meters)	1.8 m	2.0 m	1.8 m	1.8 m
Distance from obstructions on roof. Include horizontal distance + vertical height above probe for obstructions nearby. (meters)	N/A	N/A	N/A	N/A
Distance from obstructions not on roof. Include horizontal distance + vertical height above probe for obstructions nearby. (meters)	24.3 mV, 2.5mH	24.3 mV, 2.5mH	24.3 mV, 2.5mH	26.6 mV, 2.5mH
Distance from trees (meters)	26.6 m	26.6 m	26.6 m	29.5 m
Distance to furnace or incinerator flue (meters)	22.8 m	22.8 m	22.8 m	26.2 m
Distance between monitors fulfilling a QA collocation requirement (meters).	N/A	N/A	N/A	N/A
Unrestricted airflow (degrees around probe/inlet or percentage of monitoring path)	353.2	353.2	353.2	353.2
Probe material for reactive gases NO/NO <sub>2</sub> /NO <sub>y</sub> , SO <sub>2</sub> , O <sub>3</sub> ; PAMS: VOCs, Carbonyls (e.g. Pyrex, stainless steel, Teflon)	N/A	N/A	N/A	N/A
Residence time for reactive gases NO/NO <sub>2</sub> /NO <sub>y</sub> , SO <sub>2</sub> , O <sub>3</sub> ; PAMS: VOCs, Carbonyls (seconds)	N/A	N/A	N/A	N/A
Frequency of one-point QC check for gaseous instruments	N/A	N/A	N/A	N/A

Pollutant	PM10 LC	PM10 STP	PM10 STP	PM10 STP / LC
Frequency of flow rate verification for manual PM samplers, including Pb samplers (routine checks)	N/A	N/A	Monthly	N/A
Frequency of flow rate verification for automated PM analyzers (routine checks)	Biweekly	Biweekly	N/A	Biweekly
For low volume PM instruments (flow rate < 200 liters/minute), is any PM instrument within 1 m of the lovol? If yes, please list distance (meters) and instrument(s).	No	No	No	No
For high volume PM instrument (flow rate > 200 liters/minute), is any PM instrument within 2m of the hivol? If yes, please list distance (meters) and instrument(s).	No	No	No	No
Date of Annual Performance Evaluation conducted in the past calendar year for gaseous parameters (MM/DD/YYYY)	N/A	N/A	N/A	N/A
Date of two semi-annual flow rate audits conducted in the past calendar year for PM monitors (MM/DD/YYYY, MM/DD/YYYY)	10/24/17	10/24/17	05/02/17, 10/24/17	05/02/17, 10/24/17
Changes planned within the next 18 months (Y/N)	N	N	N	N

<b>Site Name</b>	<b>Corcoran-Patterson</b>
<b>AQS ID (XX-XXX-XXXX)</b>	06-031-0004
<b>Representative statistical area Name (i.e. MSA, CBSA, other)</b>	Hanford-Corcoran
<b>County</b>	Kings
<b>Collecting (Operating) Agency</b>	SJVAPCD
<b>Analytical Lab (i.e. weigh lab, toxics lab, other)</b>	CARB: PM2.5 FRM
<b>Reporting Agency</b>	CARB: PM2.5 FRM   SJVAPCD: PM2.5 FEM, PM10 FEM, Meteorology
<b>Site Start Date</b>	10/1/1996
<b>Pollutant Parameters</b>	PM2.5 FRM, PM2.5 FEM, PM10 FEM
<b>Meteorological Parameters</b>	Wind speed, wind direction, outdoor temperature
<b>Address</b>	1520 Patterson Ave., Corcoran, CA 93212
<b>GPS Coordinates (decimal degrees)</b>	36.1022 N, -119.5660 W
<b>Distance to roadways (meters)</b>	30 m (east)
<b>Traffic Count/Year</b>	3,050/2016 (Traffic count for nearest roads: JCT. Rte 43/Rte 137, Source: Caltrans 2016.)
<b>Groundcover (e.g. paved, vegetative, dirt, sand, gravel)</b>	Dirt, gravel

Corcoran-Patterson (1)					
Pollutant	PM2.5	PM2.5	PM10 LC	PM10 STP	Meteorology
Parameter code	88101	88101	85101	81102	Many
Spatial scale	N	N	N	N	N
Site type	HC	HC, PE	HC, PE	HC, PE	GB
Basic monitoring objective(s)	NC, RS	NC, RS, TP	RS, TP	NC, RS, TP	RS, TP
Monitor type	SLAMS	SLAMS	Other	SLAMS	Other
Network affiliation(s), if applicable (a monitor may have none, one, or multiple)	None	None	None	None	None
FRM/FEM/ARM/Other	FRM	FEM	FEM	FEM	Other
POC	1	3	7	7	1
Primary / QA Collocated / Other (provide for all PM <sub>2.5</sub> , PM <sub>10</sub> , PM <sub>10-2.5</sub> , Pb and NO <sub>2</sub> monitors. Non-PM, Pb, NO <sub>2</sub> monitors should be listed as "N/A".)	Primary	Other	Other	Primary	Other
Is it suitable for comparison against the annual PM <sub>2.5</sub> ? (Y/N)	Y	Y	N	N	N/A
Instrument manufacturer and model	Thermo Partisol 2025i	Teledyne 602	Teledyne 602	Teledyne 602	ITP- Hampshire Controls Corp. 125-50HLV, OT- Met One 060A-2, WD- Met One 020C, WS-Met One 010C
Analysis method	Gravimetric	Beta Attenuation	Beta Attenuation	Beta Attenuation	Many
Method code	145	204	205	205	Many
Monitoring start date (MM/DD/YYYY)	01/01/2016	01/01/2017	01/01/2017	01/01/2017	01/01/2017
Required sampling frequency (e.g. 1:3 excluding exceptional events/1:1 including exceptional events)	1:3	Hourly	Hourly	Hourly	Hourly
Sampling season (MM/DD - MM/DD)	01/01 – 12/31	01/01 – 12/31	01/01 – 12/31	01/01 – 12/31	01/01 – 12/31
Probe height (meters)	6.3 m	6.2 m	6.6 m	6.6 m	5.6 m

Pollutant	PM2.5	PM2.5	PM10 LC	PM10 STP	Meteorology
Distance from supporting structure (meters)	2.1 m	2.0 m	2.4 m	2.4 m	N/A
Distance from obstructions on roof. Include horizontal distance + vertical height above probe for obstructions nearby. (meters)	N/A	N/A	N/A	N/A	N/A
Distance from obstructions not on roof. Include horizontal distance + vertical height above probe for obstructions nearby. (meters)	115.7 m H, 1.5 m V	118.1 m H, 1.5 m V	118.1 m H, 1.5 m V	118.11 m H, 1.5 m V	118.6 m H, 1.5 m V
Distance from trees (meters)	62.5 m E 65.2 m S	63.7 m E, 65.9 m S	63.7 m E, 65.9 m S	63.7 m E, 65.9 m S	65.5 m E, 66.3 m S
Distance to furnace or incinerator flue (meters)	79.1 m	76.6 m	76.6 m	76.6 m	76.8 m
Distance between monitors fulfilling a QA collocation requirement (meters).	2.7 m	2.7 m	2.9 m	2.9 m	N/A
Unrestricted airflow (degrees around probe/inlet or percentage of monitoring path)	365	365	365	365	365
Probe material for reactive gases NO/NO <sub>2</sub> /NO <sub>y</sub> , SO <sub>2</sub> , O <sub>3</sub> ; PAMS: VOCs, Carbonyls (e.g. Pyrex, stainless steel, Teflon)	N/A	N/A	N/A	N/A	N/A
Residence time for reactive gases NO/NO <sub>2</sub> /NO <sub>y</sub> , SO <sub>2</sub> , O <sub>3</sub> ; PAMS: VOCs, Carbonyls (seconds)	N/A	N/A	N/A	N/A	N/A
Frequency of one-point QC check for gaseous instruments	N/A	N/A	N/A	N/A	N/A
Frequency of flow rate verification for manual PM samplers, including Pb samplers (routine checks)	Monthly	N/A	N/A	N/A	N/A

Pollutant	PM2.5	PM2.5	PM10 LC	PM10 STP	Meteorology
Frequency of flow rate verification for automated PM analyzers (routine checks)	N/A	Biweekly	Biweekly	Biweekly	N/A
For low volume PM instruments (flow rate < 200 liters/minute), is any PM instrument within 1 m of the hivol? If yes, please list distance (meters) and instrument(s).	No.	No.	No	No.	N/A
For high volume PM instrument (flow rate > 200 liters/minute), is any PM instrument within 2m of the hivol? If yes, please list distance (meters) and instrument(s).	N/A	N/A	N/A	N/A	N/A
Date of Annual Performance Evaluation conducted in the past calendar year for gaseous parameters (MM/DD/YYYY)	N/A	N/A	N/A	N/A	N/A
Date of two semi-annual flow rate audits conducted in the past calendar year for PM monitors (MM/DD/YYYY, MM/DD/YYYY)	5/15/17, 11/14/17	5/15/17, 11/14/17	5/15/17, 11/14/17	5/15/17, 11/14/17	N/A
Changes planned within the next 18 months (Y/N)	N	N	N	N	N

<b>Site Name</b>	<b>Visalia - Airport</b>
<b>AQS ID (XX-XXX-XXXX)</b>	06-107-3000
<b>Representative statistical area Name (i.e. MSA, CBSA, other)</b>	Visalia-Porterville
<b>County</b>	Tulare
<b>Collecting (Operating) Agency</b>	SJVAPCD
<b>Analytical Lab (i.e. weigh lab, toxics lab, other)</b>	N/A
<b>Reporting Agency</b>	SJVAPCD
<b>Site Start Date</b>	07/01/98
<b>Pollutant Parameters</b>	None
<b>Meteorological Parameters</b>	Wind speed, wind direction, outdoor temperature, relative humidity, barometric pressure, solar radiation, radio acoustic sounding system (RASS)
<b>Address</b>	9501 West Airport Drive, Visalia, CA 93277
<b>GPS Coordinates (decimal degrees)</b>	39.3266 N, -119.3984 W
<b>Distance to roadways (meters)</b>	100m (west)
<b>Traffic Count/Year</b>	65,000/2016 (Traffic count for nearest roads: JCT. Rte 99/Rte 198 East., Source: Caltrans 2016.)
<b>Groundcover (e.g. paved, vegetative, dirt, sand, gravel)</b>	Dirt, vegetative



Visalia – Airport (1)	
Pollutant	Meteorology
Parameter code	Many
Spatial scale	R
Site type	GB
Basic monitoring objective(s)	RS, TP
Monitor type	Other
Network affiliation(s), if applicable (a monitor may have none, one, or multiple)	PAMS
FRM/FEM/ARM/Other	Other
POC	1
Primary / QA Collocated / Other (provide for all PM <sub>2.5</sub> , PM <sub>10</sub> , PM <sub>10-2.5</sub> , Pb and NO <sub>2</sub> monitors. Non-PM, Pb, NO <sub>2</sub> monitors should be listed as “N/A”.)	Other
Is it suitable for comparison against the annual PM <sub>2.5</sub> ? (Y/N)	N/A
Instrument manufacturer and model	ITP- Hy-Cal 512AA3B, OT- Met One 060A-2, BP- Met One 092, RH- Vaisala HMP45D, SRD- Epply Mod. 8-48WD- Met One 020C, WS-Met One 010C
Analysis method	Many
Method code	Many
Monitoring start date (MM/DD/YYYY)	07/01/1998
Required sampling frequency (e.g. 1:3 excluding exceptional events/1:1 including exceptional events)	Hourly
Sampling season (MM/DD - MM/DD)	01/01 – 12/31
Probe height (meters)	9.8 m
Distance from supporting structure (meters)	9.8 m
Distance from obstructions on roof. Include horizontal distance + vertical height above probe for obstructions nearby. (meters)	None
Distance from obstructions not on roof. Include horizontal distance + vertical height above probe for obstructions nearby. (meters)	50.9m H 0.0m V
Distance from trees (meters)	6.1 m
Distance to furnace or incinerator flue (meters)	N/A
Distance between monitors fulfilling a QA collocation requirement (meters).	N/A
Unrestricted airflow (degrees around probe/inlet or percentage of monitoring path)	270

Pollutant	Meteorology
Probe material for reactive gases NO/NO <sub>2</sub> /NO <sub>y</sub> , SO <sub>2</sub> , O <sub>3</sub> ; PAMS: VOCs, Carbonyls (e.g. Pyrex, stainless steel, Teflon)	N/A
Residence time for reactive gases NO/NO <sub>2</sub> /NO <sub>y</sub> , SO <sub>2</sub> , O <sub>3</sub> ; PAMS: VOCs, Carbonyls (seconds)	N/A
Frequency of one-point QC check for gaseous instruments	N/A
Frequency of flow rate verification for manual PM samplers, including Pb samplers (routine checks)	N/A
Frequency of flow rate verification for automated PM analyzers (routine checks)	N/A
For low volume PM instruments (flow rate < 200 liters/minute), is any PM instrument within 1 m of the level? If yes, please list distance (meters) and instrument(s).	N/A
For high volume PM instrument (flow rate > 200 liters/minute), is any PM instrument within 2m of the level? If yes, please list distance (meters) and instrument(s).	N/A
Date of Annual Performance Evaluation conducted in the past calendar year for gaseous parameters (MM/DD/YYYY)	N/A
Date of two semi-annual flow rate audits conducted in the past calendar year for PM monitors (MM/DD/YYYY, MM/DD/YYYY)	N/A
Changes planned within the next 18 months (Y/N)	Yes. Lower air profiler at site may cease operation and be completely shut down due to changes to PAMS program requirements.

<b>Site Name</b>	<b>Visalia – Church St</b>
<b>AQS ID (XX-XXX-XXXX)</b>	06-107-2002
<b>Representative statistical area Name (i.e. MSA, CBSA, other)</b>	Visalia–Porterville
<b>County</b>	Tulare
<b>Collecting (Operating) Agency</b>	CARB
<b>Analytical Lab (i.e. weigh lab, toxics lab, other)</b>	CARB
<b>Reporting Agency</b>	CARB
<b>Site Start Date</b>	1/1/1979
<b>Pollutant Parameters</b>	Ozone, PM10 FEM, PM2.5 FRM, PM2.5 FEM, PM2.5 Speciation, NO <sub>2</sub>
<b>Meteorological Parameters</b>	Wind speed, wind direction, outdoor temperature, relative humidity
<b>Address</b>	310 N. Church St., Visalia CA 93291
<b>GPS Coordinates (decimal degrees)</b>	36.3325 N, -119.2909 W
<b>Distance to road</b>	25 m (west)
<b>Traffic Count/Year</b>	6,150/2014-2015 (Traffic count for nearest roads: E. Murray Ave. between N. Court St. and N. Santa Fe St., Source: City of Visalia Traffic and Engineering, Average Daily Traffic Volumes List 2014-2015.)
<b>Ground Cover</b>	Paved

Visalia–Church St (1)				
Pollutant	Ozone	NO <sub>2</sub>	PM10 STP / LC	PM2.5
Parameter code	44201	42602	81102, 85101	88101
Spatial scale	N	N	N	N
Site type	GB	PE	PE	PE, HC
Basic monitoring objective(s)	NC, RS,TP	NC, RS, TP	NC, RS,TP / RS,TP	NC, RS
Monitor type	SLAMS	SLAMS	SLAMS	SLAMS
Network affiliation(s), if applicable (a monitor may have none, one, or multiple)	None	None	None	None
FRM/FEM/ARM/Other	FEM	FRM	FEM	FRM
POC	1	1	5	1
Primary / QA Collocated / Other (provide for all PM <sub>2.5</sub> , PM <sub>10</sub> , PM <sub>10-2.5</sub> , Pb and NO <sub>2</sub> monitors. Non-PM, Pb, NO <sub>2</sub> monitors should be listed as "N/A".)	N/A	Primary	Primary	Primary
Is it suitable for comparison against the annual PM <sub>2.5</sub> ? (Y/N)	N/A	N/A	N/A	Y
Instrument manufacturer and model	Teledyne API 400	Teledyne API 200E	Met One 1020	R&P 2025
Analysis method	UV	Gas phase Chem.	Beta attenuation	Gravimetric
Method code	087	099	122	145
Monitoring start date (MM/DD/YYYY)	1/1/1979	1/1/1979	8/1/2015	1/3/1999
Required sampling frequency (e.g. 1:3 excluding exceptional events/1:1 including exceptional events)	Hourly	Hourly	Hourly	1:3
Sampling season (MM/DD - MM/DD)	01/01 -12/31	01/01 -12/31	01/01 -12/31	01/01 -12/31
Probe/Inlet height above ground (meters)	6.7 m	6.7 m	6.2 m	5.9 m
Distance from supporting structure (meters)	2.8 m	2.8 m	2.3 m	2.1 m
Distance from obstructions on roof. Include horizontal distance + vertical height above probe for obstructions nearby. (meters)	None	None	None	None
Distance from obstructions not on roof. Include horizontal distance + vertical height above probe for obstructions nearby. (meters)	None	None	None	None
Distance from trees (meters)	None	None	None	None
Distance to furnace or incinerator flue (meters)	None	None	None	None
Distance between collocated monitors (meters)	None	None	N/A	2.3 m
Unrestricted airflow (degrees)	360	360	360	360
Probe material (Teflon, etc.)	Teflon	Teflon	N/A	N/A

Pollutant	Ozone	NO <sub>2</sub>	PM10 STP / LC	PM2.5
Residence time (seconds)	11.6	11.0	N/A	N/A
For low volume PM instruments (flow rate < 200 liters/minute), is any PM instrument within 1 m of the lovol? If yes, please list distance (meters) and instrument(s).	N/A	N/A	No	No
For high volume PM instrument (flow rate > 200 liters/minute), is any PM instrument within 2m of the hivol? If yes, please list distance (meters) and instrument(s).	N/A	N/A	N/A	N/A
Frequency of flow rate verification for manual PM samplers audit	N/A	N/A	N/A	Monthly
Frequency of flow rate verification for automated PM analyzers audit	N/A	N/A	Monthly	N/A
Frequency of one-point QC check (gaseous)	5x/week	5x/week	N/A	N/A
Last Annual Performance Evaluation (gaseous)	11/15/2017	11/15/2017	N/A	N/A
Last two semi-annual flow rate audits for PM monitors	N/A	N/A	05/02/2017, 11/15/2017	05/02/2017, 11/15/2017
Changes planned within the next 18 months (Y/N)	N	N	N	Y

Visalia – Church St (2)			
Pollutant	PM2.5	PM2.5 Speciation	Meteorology
Parameter code	88502	Many	61106, 61104, 62102, 62201, 62101
Spatial scale	N	N	R
Site type	RT, PE	PE	General
Basic monitoring objective(s)	RS, TP	RS	RS, TP
Monitor type	Other	SLAMS	SLAMS
Network affiliation(s), if applicable (a monitor may have none, one, or multiple)	None	CSN Supplemental	None
FRM/FEM/ARM/Other	Non-FEM	FRM	Other
POC	3	5	1
Primary / QA Collocated / Other (provide for all PM <sub>2.5</sub> , PM <sub>10</sub> , PM <sub>10-2.5</sub> , Pb and NO <sub>2</sub> monitors. Non-PM, Pb, NO <sub>2</sub> monitors should be listed as “N/A”.)	Primary	Primary	Other

Pollutant	PM2.5	PM2.5 Speciation	Meteorology
Is it suitable for comparison against the annual PM <sub>2.5</sub> ? (Y/N)	N	N/A	N/A
Instrument manufacturer and model	Met One 1020	Many	RM Young 81000, Visalia HMP 155
Analysis method	Beta attenuation	Many	Sonic, Instrumental
Method Code	731	Many	066, 059
Monitoring start date (MM/DD/YYYY)	11/01/2001	01/14/2002	01/01/1995
Required sampling frequency (e.g. 1:3 excluding exceptional events/1:1 including exceptional events)	Hourly	1:3	Hourly
Sampling season (MM/DD - MM/DD)	01/01 -12/31	01/01 -12/31	01/01 -12/31
Probe height (meters)	6.0 m	5.9 m	11.9 m
Distance from supporting structure (meters)	2.2 m	None	None
Distance from obstructions on roof. Include horizontal distance + vertical height above probe for obstructions nearby. (meters)	None	None	None
Distance from obstructions not on roof. Include horizontal distance + vertical height above probe for obstructions nearby. (meters)	None	None	None
Distance from trees (meters)	None	None	None
Distance to furnace or incinerator flue (meters)	None	None	None
Distance between collocated monitors (meters)	2.3 m	None	None
Unrestricted airflow (degrees)	360	360	360
Probe material (Teflon, etc.)	N/A	N/A	N/A
Residence time (seconds)	N/A	N/A	N/A
For low volume PM instruments (flow rate < 200 liters/minute), is any PM instrument within 1 m of the lovol? If yes, please list distance (meters) and instrument(s).	No	No	N/A
For high volume PM instrument (flow rate > 200 liters/minute), is any PM instrument within 2m of the hivol? If yes, please list distance (meters) and instrument(s).	N/A	N/A	N/A
Frequency of flow rate verification for manual PM samplers audit	N/A	N/A	N/A
Frequency of flow rate verification for automated PM analyzers audit	Monthly	N/A	N/A

<b>Pollutant</b>	<b>PM2.5</b>	<b>PM2.5 Speciation</b>	<b>Meteorology</b>
Frequency of one-point QC check (gaseous)	N/A	N/A	N/A
Last Annual Performance Evaluation (gaseous)	N/A	N/A	N/A
Last two semi-annual flow rate audits for PM monitors	05/02/2017, 11/15/2017	5/2/2017	N/A
Changes planned within the next 18 months (Y/N)	N	N	N

<b>Site Name</b>	<b>Porterville</b>
<b>AQS ID (XX-XXX-XXXX)</b>	06-107-2010
<b>Representative statistical area Name (i.e. MSA, CBSA, other)</b>	Visalia-Porterville
<b>County</b>	Tulare
<b>Collecting (Operating) Agency</b>	SJVAPCD
<b>Analytical Lab (i.e. weigh lab, toxics lab, other)</b>	N/A
<b>Reporting Agency</b>	SJVAPCD
<b>Site Start Date</b>	03/08/2010
<b>Pollutant Parameters</b>	Ozone, PM2.5 FEM
<b>Meteorological Parameters</b>	Wind speed, wind direction, outdoor temperature, barometric pressure
<b>Address</b>	1839 S. Newcomb St., Porterville, CA 93257
<b>GPS Coordinates (decimal degrees)</b>	36.0310 N, -119.0550 W
<b>Distance to roadways (meters)</b>	100m (south)
<b>Traffic Count/Year</b>	25,000/2016 (Ahead AADT traffic count for nearest roads: Junction SR 190/SR 65, Source: Caltrans 2016)
<b>Groundcover (e.g. paved, vegetative, dirt, sand, gravel)</b>	Paved, vegetative



Porterville (1)			
Pollutant	Ozone	PM2.5	Meteorology
Parameter code	44201	88502	Many
Spatial scale	N	N	N
Site type	HC, PE	PE	PE
Basic monitoring objective(s)	NC, RS, TP	TP	TP
Monitor type	SLAMS	SPM	Other
Network affiliation(s), if applicable (a monitor may have none, one, or multiple)	None	None	None
FRM/FEM/ARM/Other	FEM	Non-FEM	Other
POC	1	3	1
Primary / QA Collocated / Other (provide for all PM <sub>2.5</sub> , PM <sub>10</sub> , PM <sub>10-2.5</sub> , Pb and NO <sub>2</sub> monitors. Non-PM, Pb, NO <sub>2</sub> monitors should be listed as "N/A".)	N/A	Other	Other
Is it suitable for comparison against the annual PM <sub>2.5</sub> ? (Y/N)	N/A	N	N/A
Instrument manufacturer and model	Teledyne API 400E	MET One BAM 1020	ITP- Hy-Cal 512AA3B, OT- Met One 060A-2, BP- Met One 092, WD- Met One 020C, WS- Met One 010C
Analysis method	UV	Beta Attenuation	Many
Method code	087	731	Many
Monitoring start date (MM/DD/YYYY)	03/08/2010	03/08/2010	03/08/2010
Required sampling frequency (e.g. 1:3 excluding exceptional events/1:1 including exceptional events)	Hourly	Hourly	Hourly
Sampling season (MM/DD - MM/DD)	01/01 -12/31	01/01 -12/31	01/01 -12/31
Probe height (meters)	5.3 m	4.3 m	9.1 m
Distance from supporting structure (meters)	7.1 m	1.8 m	7.1 m
Distance from obstructions on roof. Include horizontal distance + vertical height above probe for obstructions nearby. (meters)	2.1 mH, 0.0mV	3.5mH, 0.0 mV	None
Distance from obstructions not on roof. Include horizontal distance + vertical height above probe for obstructions nearby. (meters)	N/A	N/A	N/A
Distance from trees (meters)	11.5 m N	14.3 m N	14.9 m N
Distance to furnace or incinerator flue (meters)	175.5 m S	174 m S	175.8 m S

<b>Pollutant</b>	<b>Ozone</b>	<b>PM2.5</b>	<b>Meteorology</b>
Distance between monitors fulfilling a QA collocation requirement (meters).	N/A	N/A	N/A
Unrestricted airflow (degrees around probe/inlet or percentage of monitoring path)	357	357	357
Probe material for reactive gases NO/NO <sub>2</sub> /NO <sub>y</sub> , SO <sub>2</sub> , O <sub>3</sub> ; PAMS: VOCs, Carbonyls (e.g. Pyrex, stainless steel, Teflon)	Teflon/Pyrex with Borosilicate	N/A	N/A
Residence time for reactive gases NO/NO <sub>2</sub> /NO <sub>y</sub> , SO <sub>2</sub> , O <sub>3</sub> ; PAMS: VOCs, Carbonyls (seconds)	7.47	N/A	N/A
Frequency of one-point QC check for gaseous instruments	Daily	N/A	N/A
Frequency of flow rate verification for manual PM samplers, including Pb samplers (routine checks)	N/A	N/A	N/A
Frequency of flow rate verification for automated PM analyzers (routine checks)	N/A	Biweekly	N/A
For low volume PM instruments (flow rate < 200 liters/minute), is any PM instrument within 1 m of the hivol? If yes, please list distance (meters) and instrument(s).	N/A	No	N/A
For high volume PM instrument (flow rate > 200 liters/minute), is any PM instrument within 2m of the hivol? If yes, please list distance (meters) and instrument(s).	N/A	N/A	N/A
Date of Annual Performance Evaluation conducted in the past calendar year for gaseous parameters (MM/DD/YYYY)	11/14/17	N/A	N/A
Date of two semi-annual flow rate audits conducted in the past calendar year for PM monitors (MM/DD/YYYY, MM/DD/YYYY)	N/A	05/16/17, 11/14/17	N/A
Changes planned within the next 18 months (Y/N)	N	N	N

<b>Site name</b>	<b>Sequoia–Ash Mountain</b>
<b>AQS ID (XX-XXX-XXXX)</b>	06-107-0009
<b>Representative statistical area Name (i.e. MSA, CBSA, other)</b>	Visalia-Porterville
<b>County</b>	Tulare
<b>Collecting (Operating) Agency</b>	All equipment operated by NPS
<b>Analytical Lab (i.e. weigh lab, toxics lab, other)</b>	N/A
<b>Reporting Agency</b>	All data reported by NPS
<b>Site Start Date</b>	07/01/1999
<b>Pollutant Parameters</b>	Ozone, PM2.5 FEM
<b>Meteorological Parameters</b>	Wind speed, wind direction, outdoor temperature, relative humidity, solar radiation
<b>Address</b>	Ash Mountain, Sequoia National Park 47050 Generals Hwy, Three Rivers, CA 93271
<b>GPS Coordinates (decimal degrees)</b>	36.4894 N, -118.8290 W
<b>Distance to road</b>	120 m (north)
<b>Traffic Count/Year</b>	1,650/2016 (Rte 198 / Sequoia National Park boundary, Source: Caltrans Back AADT 2016)
<b>Ground Cover</b>	Dirt, vegetative

<b>Sequoia–Ash Mountain (1)</b>			
<b>Pollutant</b>	<b>Ozone</b>	<b>PM2.5</b>	<b>Meteorology</b>
Parameter code	44201	88501	Many
Spatial scale	R	R	R
Site type	HC, RT	RT	GB
Monitor objective	NC, RS, TP	RS, TP	RS, TP
Monitor type	Non-EPA Federal	Non-EPA Federal	Non-EPA Federal
Network affiliation	CASTNET	IMPROVE	CASTNET
FRM/FEM/ARM/Other	Other	FEM	Other
POC	1	1	1
Primary / QA Collocated / Other (provide for all PM <sub>2.5</sub> , PM <sub>10</sub> , PM <sub>10-2.5</sub> , Pb and NO <sub>2</sub> monitors. Non-PM, Pb, NO <sub>2</sub> monitors should be listed as "N/A".)	N/A	Primary	Other
Is it suitable for comparison against the annual PM <sub>2.5</sub> ? (Y/N)	N/A	N	N/A
Instrument manufacturer and model	Thermo TECO 49, 49C	MET One BAM 1020	Many
Analysis method	UV	Beta Attenuation	Many
Method code	047	750	Many
Monitoring start date (MM/DD/YYYY)	07/01/1999	3/19/2007	10/4/2001
Required sampling frequency (e.g. 1:3 excluding exceptional events/1:1 including exceptional events)	Hourly	Hourly	Hourly
Sampling season (MM/DD - MM/DD)	01/01 – 12/31	01/01 – 12/31	01/01 – 12/31
Probe height (meters)	10 m	4 m	10 m
Distance from supporting structure (meters)	3 m	1.5 m	3 m
Distance from obstructions on roof. Include horizontal distance + vertical height above probe for obstructions nearby. (meters)	5 m	N/A	5 m
Distance from obstructions not on roof. Include horizontal distance + vertical height above probe for obstructions nearby. (meters)	N/A	N/A	N/A
Distance from trees (meters)	15 m	15 m	15 m
Distance to furnace or incinerator flue (meters)	305 m	305 m	305 m
Distance between monitors fulfilling a QA collocation requirement (meters).	3 m	3 m	3 m
Unrestricted airflow (degrees around probe/inlet or percentage of monitoring path)	360	360	360
Probe material for reactive gases NO/NO <sub>2</sub> /NO <sub>y</sub> , SO <sub>2</sub> , O <sub>3</sub> ; PAMS: VOCs, Carbonyls (e.g. Pyrex, stainless steel, Teflon)	Teflon	N/A	N/A
Residence time for reactive gases NO/NO <sub>2</sub> /NO <sub>y</sub> , SO <sub>2</sub> , O <sub>3</sub> ; PAMS: VOCs, Carbonyls (seconds)	13.4	N/A	N/A

<b>Pollutant</b>	<b>Ozone</b>	<b>PM2.5</b>	<b>Meteorology</b>
Frequency of one-point QC check for gaseous instruments	Daily	N/A	N/A
Frequency of flow rate verification for manual PM samplers, including Pb samplers (routine checks)	N/A	N/A	N/A
Frequency of flow rate verification for automated PM analyzers (routine checks)	N/A	Bi-Weekly	N/A
For low volume PM instruments (flow rate < 200 liters/minute), is any PM instrument within 1 m of the level? If yes, please list distance (meters) and instrument(s).	N/A	N/A	N/A
For high volume PM instrument (flow rate > 200 liters/minute), is any PM instrument within 2m of the level? If yes, please list distance (meters) and instrument(s).	N/A	N/A	N/A
Date of Annual Performance Evaluation conducted in the past calendar year for gaseous parameters (MM/DD/YYYY)	4/20/2018	N/A	N/A
Date of two semi-annual flow rate audits conducted in the past calendar year for PM monitors (MM/DD/YYYY, MM/DD/YYYY)	N/A	09/06/2017, 04/04/2018	N/A
Changes planned within the next 18 months (Y/N)	N	N	N

<b>Site name</b>	<b>Sequoia–Lower Kaweah</b>
<b>AQS ID (XX-XXX-XXXX)</b>	061070006
<b>Representative statistical area Name (i.e. MSA, CBSA, other)</b>	Visalia-Porterville
<b>County</b>	Tulare
<b>Collecting (Operating) Agency</b>	All equipment operated by NPS
<b>Analytical Lab (i.e. weigh lab, toxics lab, other)</b>	N/A
<b>Reporting Agency</b>	All data reported by NPS
<b>Site Start Date</b>	01/01/1987
<b>Pollutant Parameters</b>	Ozone, NADP (wet deposition)
<b>Meteorological Parameters</b>	Wind speed, wind direction, outdoor temperature, relative humidity, solar radiation
<b>Address</b>	Giant Forest, Sequoia National Park, 47050 Generals Highway, Three Rivers, CA 93271
<b>GPS Coordinates (decimal degrees)</b>	36.5661 N, -118.7776 W
<b>Distance to road</b>	380 m (southeast)
<b>Traffic Count/Year</b>	1,650/2016 (Rte 198 / Sequoia National Park boundary, Source: Caltrans Back AADT 2016)
<b>Ground Cover</b>	Dirt, vegetation

Sequoia–Lower Kaweah (1)		
Pollutant	Ozone	Meteorology
Parameter code	44201	Many
Spatial scale	R	R
Site type	RT	GB
Monitor objective	NC, RS, TP	RS, TP
Monitor type	Non-EPA Federal	Non-EPA Federal
Network affiliation	None	None
FRM/FEM/ARM/Other	Other	Other
POC	1	1
Primary / QA Collocated / Other (provide for all PM <sub>2.5</sub> , PM <sub>10</sub> , PM <sub>10-2.5</sub> , Pb and NO <sub>2</sub> monitors. Non-PM, Pb, NO <sub>2</sub> monitors should be listed as "N/A".)	N/A	Other
Is it suitable for comparison against the annual PM <sub>2.5</sub> ? (Y/N)	N/A	N/A
Instrument manufacturer and model	Thermo TECO 49, 49C	Many
Analysis method	UV	Many
Method code	047	Many
Monitoring start date (MM/DD/YYYY)	01/01/1987	04/01/1987
Required sampling frequency (e.g. 1:3 excluding exceptional events/1:1 including exceptional events)	Hourly	Hourly
Sampling season (MM/DD - MM/DD)	01/01 – 12/31	01/01 – 12/31
Probe height (meters)	5	5
Distance from supporting structure (meters)	1.5	10
Distance from obstructions on roof. Include horizontal distance + vertical height above probe for obstructions nearby. (meters)	1	N/A
Distance from obstructions not on roof. Include horizontal distance + vertical height above probe for obstructions nearby. (meters)	N/A	N/A
Distance from trees (meters)	5-10 m	5-10 m
Distance to furnace or incinerator flue (meters)	457 m	457 m
Distance between monitors fulfilling a QA collocation requirement (meters).	5-10 m	10-15 m
Unrestricted airflow (degrees around probe/inlet or percentage of monitoring path)	360	360
Probe material for reactive gases NO/NO <sub>2</sub> /NO <sub>y</sub> , SO <sub>2</sub> , O <sub>3</sub> ; PAMS: VOCs, Carbonyls (e.g. Pyrex, stainless steel, Teflon)	Teflon	N/A

Pollutant	Ozone	Meteorology
Residence time for reactive gases NO/NO <sub>2</sub> /NO <sub>y</sub> , SO <sub>2</sub> , O <sub>3</sub> ; PAMS: VOCs, Carbonyls (seconds)	13.9	N/A
Frequency of one-point QC check for gaseous instruments	Daily	N/A
Frequency of flow rate verification for manual PM samplers, including Pb samplers (routine checks)	N/A	N/A
Frequency of flow rate verification for automated PM analyzers (routine checks)	N/A	N/A
For low volume PM instruments (flow rate < 200 liters/minute), is any PM instrument within 1 m of the hivol? If yes, please list distance (meters) and instrument(s).	N/A	N/A
For high volume PM instrument (flow rate > 200 liters/minute), is any PM instrument within 2m of the hivol? If yes, please list distance (meters) and instrument(s).	N/A	N/A
Date of Annual Performance Evaluation conducted in the past calendar year for gaseous parameters (MM/DD/YYYY)	04/20/2018	N/A
Date of two semi-annual flow rate audits conducted in the past calendar year for PM monitors (MM/DD/YYYY, MM/DD/YYYY)	N/A	N/A
Changes planned within the next 18 months (Y/N)	N	N



<b>Site Name</b>	<b>Shafter</b>	
<b>AQS ID (XX-XXX-XXXX)</b>	06-029-6001	
<b>Representative statistical area Name (i.e. MSA, CBSA, other)</b>	Bakersfield	
<b>County</b>	Kern	
<b>Collecting (Operating) Agency</b>	CARB: Ozone, NO2;	SJVAPCD: Meteorology, Speciated VOC, NMH
<b>Analytical Lab (i.e. weigh lab, toxics lab, other)</b>	CARB: Ozone, NO2	Varies based on which laboratory is contracted with the SJVAPCD: Speciated VOC, NMH
<b>Reporting Agency</b>	CARB: Ozone, NO2	SJVAPCD: Speciated VOC, NMH, Meteorology
<b>Site Start Date</b>	01/01/1989	
<b>Pollutant Parameters</b>	Ozone, NO2, Speciated VOC, NMH	
<b>Meteorological Parameters</b>	Wind speed, wind direction, outdoor temperature, relative humidity, barometric pressure, solar radiation	
<b>Address</b>	578 Walker St., Shafter, CA 93263	
<b>GPS Coordinates (decimal degrees)</b>	35.5034 N, -119.2726 W	
<b>Distance to roadways (meters)</b>	10m (southwest)	
<b>Traffic Count/Year</b>	3,986/2017 (Traffic count for nearest roads: Central Ave and Walker St., Source: Kern Council of Governments.)	
<b>Groundcover (e.g. paved, vegetative, dirt, sand, gravel)</b>	Paved	

Shafter (1)					
Pollutant	Ozone	NO <sub>2</sub>	Speciated VOC	NMH	Meteorology
Parameter code	44201	42602	Many	43102	Many
Spatial scale	N	N	N	N	R
Site type	GB, PE	PE	PE	PE	GB
Basic monitoring objective(s)	NC, RS, TP	NC, RS, TP	RS	RS, TP	RS, TP
Monitor type	SLAMS	SLAMS	Other	Other	Other
Network affiliation(s), if applicable (a monitor may have none, one, or multiple)	PAMS	PAMS	PAMS	PAMS	PAMS
FRM/FEM/ARM/Other	FEM	FRM	Other	Other	Other
POC	1	1	1	1	1
Primary / QA Collocated / Other (provide for all PM <sub>2.5</sub> , PM <sub>10</sub> , PM <sub>10-2.5</sub> , Pb and NO <sub>2</sub> monitors. Non-PM, Pb, NO <sub>2</sub> monitors should be listed as "N/A".)	N/A	N/A	Other	Other	Other
Is it suitable for comparison against the annual PM <sub>2.5</sub> ? (Y/N)	N/A	N/A	N/A	N/A	N/A
Instrument manufacturer and model	Teledyne 400E	Teledyne API 200E	Xontech 910A	Synspec Alpha 115	ITP- Hy-Cal BA512AA3BB, OT- Met One 060A-2, SRD- Epply Mod. 8-48, WD- Met One 020B, WS- Met One 010C, BP- Met One 092
Analysis method	UV	CL	GC	GC	Many
Method code	087	099	164	011	Many
Monitoring start date (MM/DD/YYYY)	07/01/1989	07/01/1989	07/01/1994	07/01/1994	01/01/1989
Required sampling frequency (e.g. 1:3 excluding exceptional events/1:1 including exceptional events)	Hourly	Hourly	1:3	Hourly	Hourly
Sampling season (MM/DD - MM/DD)	01/01 – 12/31	01/01 – 12/31	06/01 – 08/31	01/01 – 12/31	01/01 – 12/31
Probe height (meters)	7.3 m	7.3 m	7.0 m	7.0 m	10 m
Distance from supporting structure (meters)	2.6 m	2.6 m	2.4 m	2.4 m	None
Distance from obstructions on roof. Include horizontal distance + vertical height above probe for obstructions nearby. (meters)	None	None	None	None	None

Pollutant	Ozone	NO <sub>2</sub>	Speciated VOC	NMH	Meteorology
Distance from obstructions not on roof. Include horizontal distance + vertical height above probe for obstructions nearby. (meters)	None	None	19m H, 2m V (Tree)	19m H, 2m V (Tree)	N/A
Distance from trees (meters)	None	None	19m N, 70m SE	19m N, 70m SE	70m SE
Distance to furnace or incinerator flue (meters)	None	None	N/A	N/A	N/A
Distance between monitors fulfilling a QA collocation requirement (meters).	None	None	N/A	N/A	N/A
Unrestricted airflow (degrees around probe/inlet or percentage of monitoring path)	360	360	355	350	360
Probe material for reactive gases NO/NO <sub>2</sub> /NO <sub>y</sub> , SO <sub>2</sub> , O <sub>3</sub> ; PAMS: VOCs, Carbonyls (e.g. Pyrex, stainless steel, Teflon)	Teflon/Pyrex with Borosilicate	Teflon/Pyrex with Borosilicate	Stainless Steel	Teflon/Pyrex with Borosilicate	N/A
Residence time for reactive gases NO/NO <sub>2</sub> /NO <sub>y</sub> , SO <sub>2</sub> , O <sub>3</sub> ; PAMS: VOCs, Carbonyls (seconds)	10.3	11.7	2.79	< 14 sec.	N/A
Frequency of one-point QC check for gaseous instruments	Daily	Daily	N/A	Daily	N/A
Frequency of flow rate verification for manual PM samplers, including Pb samplers (routine checks)	N/A	N/A	N/A	N/A	N/A
Frequency of flow rate verification for automated PM analyzers (routine checks)	N/A	N/A	N/A	N/A	N/A
For low volume PM instruments (flow rate < 200 liters/minute), is any PM instrument within 1 m of the hivol? If yes, please list distance (meters) and instrument(s).	N/A	N/A	N/A	N/A	N/A
For high volume PM instrument (flow rate > 200 liters/minute), is any PM instrument within 2m of the hivol? If yes, please list distance (meters) and instrument(s).	N/A	N/A	N/A	N/A	N/A
Date of Annual Performance Evaluation conducted in the past calendar year for gaseous parameters (MM/DD/YYYY)	11/01/2017	11/01/2017	N/A	N/A	N/A
Date of two semi-annual flow rate audits conducted in the past calendar year for PM monitors (MM/DD/YYYY, MM/DD/YYYY)	N/A	N/A	N/A	N/A	N/A
Changes planned within the next 18 months (Y/N)	N	N	N	N	N

<b>Site Name</b>	<b>Oildale</b>
<b>AQS ID (XX-XXX-XXXX)</b>	06-029-0232
<b>Representative statistical area Name (i.e. MSA, CBSA, other)</b>	Bakersfield
<b>County</b>	Kern
<b>Collecting (Operating) Agency</b>	CARB
<b>Analytical Lab (i.e. weigh lab, toxics lab, other)</b>	CARB
<b>Reporting Agency</b>	CARB
<b>Site Start Date</b>	01/01/1980
<b>Pollutant Parameters</b>	Ozone, PM10 FEM
<b>Meteorological Parameters</b>	Wind speed, wind direction, outdoor temperature, sonic temperature, relative humidity
<b>Address</b>	3311 Manor St, Oildale CA 93308
<b>GPS Coordinates (decimal degrees)</b>	35.4380 N, -119.0167 W
<b>Distance to road</b>	150 m (northwest)
<b>Traffic Count/Year</b>	7,569/2018 (Traffic count for roads: Manor St. between Day Ave and Felton St., Source: Kern Council of Governments.)
<b>Ground Cover</b>	Dirt, vegetative

Oildale (1)				
Pollutant	Ozone	PM10 STP	PM10 STP / LC	Meteorology
Parameter code	44201	81102	81102, 85101	Many
Spatial scale	U	MD	MD	U
Site type	HC, RT	SO	SO	GB
Basic monitoring objective(s)	NC, RS, TP	NC, RS	NC, RS, TP	NC
Monitor type	SLAMS	SLAMS	SLAMS	SLAMS
Network affiliation(s), if applicable (a monitor may have none, one, or multiple)	None	None	None	None
FRM/FEM/ARM/Other	FEM	FRM	FEM	Other
POC	1	2	3	Many
Primary / QA Collocated / Other (provide for all PM <sub>2.5</sub> , PM <sub>10</sub> , PM <sub>10-2.5</sub> , Pb and NO <sub>2</sub> monitors. Non-PM, Pb, NO <sub>2</sub> monitors should be listed as "N/A".)	Primary	Primary	Primary	Other
Is it suitable for comparison against the annual PM <sub>2.5</sub> ? (Y/N)	N/A	N/A	N/A	N/A
Instrument manufacturer and model	Teledyne API 400	Sierra Anderson 1200	MET One BAM 1020	RM Young 81000, Vaisala HMP 155
Analysis method	UV	Gravimetric	Beta Attenuation	Many
Method code	087	063	122	Many
Monitoring start date (MM/DD/YYYY)	01/01/1984	01/01/1987 End date: 05/31/2017	06/01/2017	01/01/1999, 03/0620/04, 10/01/2005
Required sampling frequency (e.g. 1:3 excluding exceptional events/1:1 including exceptional events)	Hourly	1:6	Hourly	Hourly
Sampling season (MM/DD - MM/DD)	01/01 – 12/31	01/01 – 12/31	01/01 – 12/31	01/01 – 12/31
Probe/Inlet height above ground (meters)	6.7 m	2.2 m	2.2 m	8.5 m
Distance from supporting structure (meters)	3.0 m	1.5 m	1.5 m	1.3 m
Distance from obstructions on roof. Include horizontal distance + vertical height above probe for obstructions nearby. (meters)	N/A	N/A	N/A	N/A
Distance from obstructions not on roof. Include horizontal distance + vertical height above probe for obstructions nearby. (meters)	N/A	N/A	N/A	N/A

Pollutant	Ozone	PM10 STP	PM10 STP / LC	Meteorology
Distance from trees (meters)	10.1 m	N/A	N/A	N/A
Distance to furnace or incinerator flue (meters)	N/A	N/A	N/A	N/A
Distance between collocated monitors (meters)	N/A	N/A	N/A	N/A
Unrestricted airflow (degrees)	360	360	360	360
Probe material (Teflon, etc.)	Teflon	N/A	N/A	N/A
Residence time (seconds)	12.4	N/A	N/A	N/A
For low volume PM instruments (flow rate < 200 liters/minute), is any PM instrument within 1 m of the lovol? If yes, please list distance (meters) and instrument(s).	N/A	N/A	N/A	N/A
For high volume PM instrument (flow rate > 200 liters/minute), is any PM instrument within 2m of the hivol? If yes, please list distance (meters) and instrument(s).	N/A	No	No	N/A
Frequency of flow rate verification for manual PM samplers audit	N/A	Monthly	N/A	N/A
Frequency of flow rate verification for automated PM analyzers audit	N/A	N/A	Bi-Monthly	N/A
Frequency of one-point QC check (gaseous)	Daily	N/A	N/A	N/A
Last Annual Performance Evaluation (gaseous)	3/23/2017	N/A	N/A	N/A
Last two semi-annual flow rate audits for PM monitors	N/A	03/23/2017	09/20/2017, 03/08/2018	N/A
Changes planned within the next 18 months (Y/N)	N	Hi-vol was replaced with a BAM1020 after safety repairs were made to the station's rooftop.	N	N

<b>Site Name</b>	<b>Bakersfield – Golden/M St</b>
<b>AQS ID (XX-XXX-XXXX)</b>	06-029-0010
<b>Representative statistical area Name (i.e. MSA, CBSA, other)</b>	Bakersfield
<b>County</b>	Kern
<b>Collecting (Operating) Agency</b>	SJVAPCD
<b>Analytical Lab (i.e. weigh lab, toxics lab, other)</b>	CARB
<b>Reporting Agency</b>	CARB
<b>Site Start Date</b>	06/10/2014
<b>Pollutant Parameters</b>	PM10 FRM and PM2.5 FRM
<b>Meteorological Parameters</b>	None
<b>Address</b>	2820 M St., Bakersfield, CA 93301
<b>GPS Coordinates (decimal degrees)</b>	35.385574 N, -119.015009 W
<b>Distance to roadways (meters)</b>	13 M
<b>Traffic Count/Year</b>	4,562/2018 (Traffic count for nearest roads: 30th St. at Golden State Ave., Source: Kern Council of Governments.)
<b>Groundcover (e.g. paved, vegetative, dirt, sand, gravel)</b>	Paved

<b>Bakersfield – Golden/M St (1)</b>		
<b>Pollutant</b>	<b>PM2.5</b>	<b>PM10 STP</b>
Parameter code	88101	81102
Spatial scale	MC	MC
Site type	PE	PE
Basic monitoring objective(s)	NC, RS	NC, RS
Monitor type	SLAMS	SLAMS
Network affiliation(s), if applicable (a monitor may have none, one, or multiple)	None	None
FRM/FEM/ARM/Other	FRM	FRM
POC	1	1
Primary / QA Collocated / Other (provide for all PM <sub>2.5</sub> , PM <sub>10</sub> , PM <sub>10-2.5</sub> , Pb and NO <sub>2</sub> monitors. Non-PM, Pb, NO <sub>2</sub> monitors should be listed as "N/A".)	Primary	Primary
Is it suitable for comparison against the annual PM <sub>2.5</sub> ? (Y/N)	Y	N/A
Instrument manufacturer and model	Thermo 2025i	Hi Vol SSI Ecotech Model 3000
Analysis method	Gravimetric	Gravimetric
Method code	145	162
Monitoring start date (MM/DD/YYYY)	07/02/2014	04/01/2015
Required sampling frequency (e.g. 1:3 excluding exceptional events/1:1 including exceptional events)	1:3	1:6
Sampling season (MM/DD - MM/DD)	01/01 – 12/31	01/01 – 12/31
Probe height (meters)	6.2 m	5.9 m
Distance from supporting structure (meters)	2.1 m	1.8 m
Distance from obstructions on roof. Include horizontal distance + vertical height above probe for obstructions nearby. (meters)	N/A	N/A
Distance from obstructions not on roof. Include horizontal distance + vertical height above probe for obstructions nearby. (meters)	N/A	N/A
Distance from trees (meters)	11m WSW	12m WSW
Distance to furnace or incinerator flue (meters)	N/A	N/A
Distance between monitors fulfilling a QA collocation requirement (meters).	N/A	N/A
Unrestricted airflow (degrees around probe/inlet or percentage of monitoring path)	340	340
Probe material for reactive gases NO/NO <sub>2</sub> /NO <sub>y</sub> , SO <sub>2</sub> , O <sub>3</sub> ; PAMS: VOCs, Carbonyls (e.g. Pyrex, stainless steel, Teflon)	N/A	N/A



Pollutant	PM2.5	PM10 STP
Residence time for reactive gases NO/NO <sub>2</sub> /NO <sub>y</sub> , SO <sub>2</sub> , O <sub>3</sub> ; PAMS: VOCs, Carbonyls (seconds)	N/A	N/A
Frequency of one-point QC check for gaseous instruments	N/A	N/A
Frequency of flow rate verification for manual PM samplers, including Pb samplers (routine checks)	Monthly	Monthly
Frequency of flow rate verification for automated PM analyzers (routine checks)	N/A	N/A
For low volume PM instruments (flow rate < 200 liters/minute), is any PM instrument within 1 m of the lovol? If yes, please list distance (meters) and instrument(s).	No	No
For high volume PM instrument (flow rate > 200 liters/minute), is any PM instrument within 2m of the hivol? If yes, please list distance (meters) and instrument(s).	No	No
Date of Annual Performance Evaluation conducted in the past calendar year for gaseous parameters (MM/DD/YYYY)	N/A	N/A
Date of two semi-annual flow rate audits conducted in the past calendar year for PM monitors (MM/DD/YYYY, MM/DD/YYYY)	03/22/17; 09/21/17	03/22/17; 09/21/17
Changes planned within the next 18 months (Y/N)	N	N

<b>Site Name</b>	<b>Bakersfield–California</b>
<b>AQS ID (XX-XXX-XXXX)</b>	06-029-0014
<b>Representative statistical area Name (i.e. MSA, CBSA, other)</b>	Bakersfield
<b>County</b>	Kern
<b>Collecting (Operating) Agency</b>	CARB
<b>Analytical Lab (i.e. weigh lab, toxics lab, other)</b>	CARB
<b>Reporting Agency</b>	CARB
<b>Site Start Date</b>	03/01/1994
<b>Pollutant Parameters</b>	Ozone, PM10 FRM, PM2.5 FRM, PM2.5 Non-FEM, NO <sub>2</sub> , Toxics, PM2.5 Speciation (STN)
<b>Meteorological Parameters</b>	Wind speed, wind direction, outdoor temperature, sonic temperature, relative humidity
<b>Address</b>	5558 California Ave., Bakersfield CA 93309
<b>GPS Coordinates (decimal degrees)</b>	35.3566 N, -119.0626 W
<b>Distance to road</b>	300 m (south)
<b>Traffic Count/Year</b>	33,244/2017 (Traffic count for roads: California Ave between Stockdale Hwy and Business Center Dr., Source: Kern Council of Governments.)
<b>Ground Cover</b>	Paved

<b>Bakersfield – California (1)</b>					
<b>Pollutant</b>	<b>Ozone</b>	<b>PM10 STP</b>	<b>PM10 STP</b>	<b>PM2.5</b>	<b>PM2.5</b>
Parameter code	44201	81102	81102	88101	88101
Spatial scale	N	N	N	N	N
Site type	HC, GB	PE	PE, QA	HC, PE	HC, PE, QA
Basic monitoring objective(s)	NC, RS, TP	NC, RS	NC, RS	NC, RS	NC, RS
Monitor type	SLAMS	SLAMS	SLAMS	SLAMS	SLAMS
Network affiliation(s), if applicable (a monitor may have none, one, or multiple)	None	None	None	None	None
FRM/FEM/ARM/Other	FEM	FRM	FRM	FRM	FRM
POC	1	1	2	1	2
Primary / QA Collocated / Other (provide for all PM <sub>2.5</sub> , PM <sub>10</sub> , PM <sub>10-2.5</sub> , Pb and NO <sub>2</sub> monitors. Non-PM, Pb, NO <sub>2</sub> monitors should be listed as "N/A".)	N/A	Primary	QA Collocated	Primary	QA Collocated
Is it suitable for comparison against the annual PM <sub>2.5</sub> ? (Y/N)	N/A	N/A	N/A	Y	Y
Instrument manufacturer and model	Teledyne API 400E	SA/GMW 1200	SA/GMW 1200	Thermo 2025i	Thermo 2025i
Analysis method	UV	Gravimetric	Gravimetric	Gravimetric	Gravimetric
Method code	087	063	063	145	145
Monitoring start date (MM/DD/YYYY)	3/1/1994	4/1/1994	1/3/2003	1/1/1999	1/1/1999
Required sampling frequency (e.g. 1:3 excluding exceptional events/1:1 including exceptional events)	Hourly	1:6	1:12	1:1	1:12
Sampling season (MM/DD - MM/DD)	01/01 – 12/31	01/01 – 12/31	01/01 – 12/31	01/01 – 12/31	01/01 – 12/31
Probe/Inlet height above ground (meters) (ground to rooftop = 4.1m)	7.2 m	5.62 m	5.62 m	6.23 m	6.23 m
Distance from supporting structure (above rooftop) (meters)	3.1 m	1.52 m	1.52 m	2.13 m	2.13 m

Pollutant	Ozone	PM10 STP	PM10 STP	PM2.5	PM2.5
Distance from obstructions on roof. Include horizontal distance + vertical height above probe for obstructions nearby. (meters)	5.5 m rooftop access	7 m rooftop access	10 m rooftop access	None	None
Distance from obstructions not on roof. Include horizontal distance + vertical height above probe for obstructions nearby. (meters)	1.2 mH x 4.37 mD parapet	None	None	1.2 mH x 3.12 mD parapet	1.2 mH x 3.12 mD parapet
Distance from trees (meters)	>10 m	10.5 m	10 m	9.5 m	11.5 m
Distance to furnace or incinerator flue (meters)	3 m	3 m	2.8 m	2.7 m	3.5 m
Distance between collocated monitors (meters)	N/A	3.5 m	3.5 m	2.3 m	2.3 m
Unrestricted airflow (degrees)	360	360	360	360	360
Probe material (Teflon, etc.)	Teflon	N/A	N/A	N/A	N/A
Residence time (seconds)	11.58	N/A	N/A	N/A	N/A
For low volume PM instruments (flow rate < 200 liters/minute), is any PM instrument within 1 m of the level? If yes, please list distance (meters) and instrument(s).	N/A	N/A	N/A	No	No
For high volume PM instrument (flow rate > 200 liters/minute), is any PM instrument within 2m of the level? If yes, please list distance (meters) and instrument(s).	N/A	No	No	N/A	N/A
Frequency of flow rate verification for manual PM samplers audit	N/A	Monthly	Monthly	Monthly	Monthly
Frequency of flow rate verification for automated PM analyzers audit	N/A	N/A	N/A	N/A	N/A

Pollutant	Ozone	PM10 STP	PM10 STP	PM2.5	PM2.5
Frequency of one-point QC check (gaseous)	Daily	N/A	N/A	N/A	N/A
Last Annual Performance Evaluation (gaseous)	3/21/2017	N/A	N/A	N/A	N/A
Last two semi-annual flow rate audits for PM monitors	N/A	08/08/2017 02/16/2018	08/08/2017 02/16/2018	05/12/2017, 11/22/2017	11/16/2017, 02/16/2018
Changes planned within the next 18 months (Y/N)	N	N	N	N	N

Bakersfield – California (2)				
Pollutant	PM2.5	PM2.5 Speciation	PM2.5 Speciation	PM2.5 Speciation
Parameter code	88502	88356	Many	Many
Spatial scale	N	N,U	N,U	N,U
Site type	PE	PE, QA	PE	PE, QA
Basic monitoring objective(s)	RS, TP	RS	RS	RS
Monitor type	Other	SLAMS	Other	Other
Network affiliation(s), if applicable (a monitor may have none, one, or multiple)	None	STN	CSN STN	CSN STN
FRM/FEM/ARM/Other	Non-FEM	Other	Other	Other
POC	3	6	5	6
Primary / QA Collocated / Other (provide for all PM <sub>2.5</sub> , PM <sub>10</sub> , PM <sub>10-2.5</sub> , Pb and NO <sub>2</sub> monitors. Non-PM, Pb, NO <sub>2</sub> monitors should be listed as "N/A".)	Primary	Primary & QA Collocated	Primary	QA Collocated
Is it suitable for comparison against the annual PM <sub>2.5</sub> ? (Y/N)	N	N/A	N/A	N/A
Instrument manufacturer and model	Met One BAM 1020	URG 3000-N	Met One SASS	Met One SASS
Analysis method	Beta Attenuation	Cyclone inlet	Many	Many
Method code	731	839	810	810
Monitoring start date (MM/DD/YYYY)	11/01/2001	05/03/2007	01/01/2001	01/01/2001

Pollutant	PM2.5	PM2.5 Speciation	PM2.5 Speciation	PM2.5 Speciation
Required sampling frequency (e.g. 1:3 excluding exceptional events/1:1 including exceptional events)	Hourly	Primary = 1:3 / Collocated = 1:6	1:3	1:6
Sampling season (MM/DD - MM/DD)	01/01 – 12/31	01/01 – 12/31	01/01 – 12/31	
Probe/Inlet height above ground (meters)	6.43 m	6.15 m	5.95 m	5.95 m
Distance from supporting structure (meters)	2.33 m	2.05 m	1.85 m	1.85 m
Distance from obstructions on roof. Include horizontal distance + vertical height above probe for obstructions nearby. (meters)	5 m rooftop access	11 m & 13 m rooftop access	7.5 m rooftop access	9.5 m rooftop access
Distance from obstructions not on roof. Include horizontal distance + vertical height above probe for obstructions nearby. (meters)	1.2 mH x 4.37 mD	Parapet height of 1.1 m surrounding rooftop (1.2 H x 7.0 D)	1.2 mH x 7.0 mD	1.2 mH x 7.0 mD
Distance from trees (meters)	8.5 m	7 m & 9 m	7 m	8 m
Distance to furnace or incinerator flue (meters)	1.5 m	5 m & 7 m	5 m	6 m
Distance between collocated monitors (meters)	N/A	1.5 m & 1.5 m	2 m	2 m
Unrestricted airflow (degrees)	360	360 & 360	360	360
Probe material (Teflon, etc.)	N/A	N/A	N/A	N/A
Residence time (seconds)	N/A	N/A	N/A	N/A
For low volume PM instruments (flow rate < 200 liters/minute), is any PM instrument within 1 m of the level? If yes, please list distance (meters) and instrument(s).	N/A	N/A	N/A	N/A

Pollutant	PM2.5	PM2.5 Speciation	PM2.5 Speciation	PM2.5 Speciation
For high volume PM instrument (flow rate > 200 liters/minute), is any PM instrument within 2m of the hivol? If yes, please list distance (meters) and instrument(s).	N/A	N/A	N/A	N/A
Frequency of flow rate verification for manual PM samplers audit	N/A	Monthly	Monthly	Monthly
Frequency of flow rate verification for automated PM analyzers audit	Monthly	N/A	N/A	N/A
Frequency of one-point QC check (gaseous)	N/A	N/A	N/A	N/A
Last Annual Performance Evaluation (gaseous)	N/A	N/A	N/A	N/A
Last two semi-annual flow rate audits for PM monitors	07/20/2017, 02/16/2018	P 09/18/2017 C 07/14/2017	01/09/2017 07/20/2017	03/22/2017 09/07/2017
Changes planned within the next 18 months (Y/N)	N	N	N	N

Bakersfield – California (3)				
Pollutant	NO <sub>2</sub>	Toxics	Toxics	Meteorology
Parameter code	42602	Many	Many	61103, 61104, 62102, 62201, 62101
Spatial scale	N	N	N	R
Site type	PE	PE	PE, QA	GB
Basic monitoring objective(s)	NC, RS, TP	RS, TP	RS, TP	RS, TP
Monitor type	SLAMS	Many	Many	Many
Network affiliation(s), if applicable (a monitor may have none, one, or multiple)	None	CA Air Toxics	CA Air Toxics	SLAMS
FRM/FEM/ARM/Other	FRM	Other	Other	Other
POC	1	Many	Many	Many

Pollutant	NO <sub>2</sub>	Toxics	Toxics	Meteorology
Primary / QA Collocated / Other (provide for all PM <sub>2.5</sub> , PM <sub>10</sub> , PM <sub>10-2.5</sub> , Pb and NO <sub>2</sub> monitors. Non-PM, Pb, NO <sub>2</sub> monitors should be listed as "N/A".)	N/A	Primary	QA Collocated	Other
Is it suitable for comparison against the annual PM <sub>2.5</sub> ? (Y/N)	N/A	N/A	N/A	N/A
Instrument manufacturer and model	Teledyne API 200E	Xontech 924	Xontech 924	Many
Analysis method	CL	Many	Many	Sonic, Instrumental
Method code	099	Many	Many	Many
Monitoring start date (MM/DD/YYYY)	04/01/1994	01/01/2007	01/01/2007	04/01/1994
Required sampling frequency (e.g. 1:3 excluding exceptional events/1:1 including exceptional events)	Hourly	1:12	1:12	Hourly
Sampling season (MM/DD - MM/DD)	01/01 – 12/31	01/01 – 12/31	01/01 – 12/31	01/01 – 12/31
Probe/Inlet height above ground (meters)	7.2 m	5.7 m	5.7 m	13.8 m
Distance from supporting structure (meters)	3.1 m	1.9 m	1.9 m	N/A
Distance from obstructions on roof. Include horizontal distance + vertical height above probe for obstructions nearby. (meters)	5.5 m	7.5 m	9.5 m	N/A
Distance from obstructions not on roof. Include horizontal distance + vertical height above probe for obstructions nearby. (meters)	1.2 mH x 4.37 mD	1.2 mH x 3.89 mD	1.2 mH x 3.89 mD	N/A
Distance from trees (meters)	>10 m	14 m	15 m	N/A
Distance to furnace or incinerator flue (meters)	3 m	2 m	3 m	N/A
Distance between collocated monitors (meters)	N/A	N/A	N/A	N/A



Pollutant	NO <sub>2</sub>	Toxics	Toxics	Meteorology
Unrestricted airflow (degrees)	360	360	360	360
Probe material (Teflon, etc.)	Teflon	N/A	N/A	N/A
Residence time (seconds)	10.2	N/A	N/A	N/A
For low volume PM instruments (flow rate < 200 liters/minute), is any PM instrument within 1 m of the hivol? If yes, please list distance (meters) and instrument(s).	N/A	N/A	N/A	N/A
For high volume PM instrument (flow rate > 200 liters/minute), is any PM instrument within 2m of the hivol? If yes, please list distance (meters) and instrument(s).	N/A	N/A	N/A	N/A
Frequency of flow rate verification for manual PM samplers audit	N/A	Monthly	Monthly	N/A
Frequency of flow rate verification for automated PM analyzers audit	N/A	N/A	N/A	N/A
Frequency of one-point QC check (gaseous)	Daily	N/A	N/A	N/A
Last Annual Performance Evaluation (gaseous)	10/11/2017	N/A	N/A	N/A
Last two semi-annual flow rate audits for PM monitors	N/A	12/05/2017, 06/09/2017	12/05/2017, 06/09/2017	N/A
Changes planned within the next 18 months (Y/N)	N	N	N	N

<b>Site Name</b>	<b>Bakersfield - Muni</b>
<b>AQS ID (XX-XXX-XXXX)</b>	06-029-2012
<b>Representative statistical area Name (i.e. MSA, CBSA, other)</b>	Bakersfield
<b>County</b>	Kern
<b>Collecting (Operating) Agency</b>	SJVAPCD
<b>Analytical Lab (i.e. weigh lab, toxics lab, other)</b>	Varies based on which laboratory is contracted with the SJVAPCD: Speciated VOC
<b>Reporting Agency</b>	SJVAPCD
<b>Site Start Date</b>	06/01/2012
<b>Pollutant Parameters</b>	Ozone , CO, NO2, Speciated VOC, NMH
<b>Meteorological Parameters</b>	Wind speed, wind direction, outdoor temperature, relative humidity, barometric pressure, solar radiation
<b>Address</b>	2000 South Union Ave., Bakersfield, CA 93307
<b>GPS Coordinates (decimal degrees)</b>	35.3313 N, -119.0000 W
<b>Distance to roadways (meters)</b>	280m (west)
<b>Traffic Count/Year</b>	21,309/2017 (Traffic count for monitoring station's street address): S. Union Ave between E Casa Loma Dr and Watts Dr.) Source: Kern Council of Governments. 4,594/2017 (Traffic count for road adjacent to monitoring station: Watts Dr between S. Union Ave and Short St.) Source: Kern Council of Governments.
<b>Groundcover (e.g. paved, vegetative, dirt, sand, gravel)</b>	Paved

Bakersfield – Muni (1)						
Pollutant	Ozone	CO	NO <sub>2</sub>	Speciated VOC	NMH	Meteorology
Parameter code	44201	42101	42602	Many	43102	Many
Spatial scale	N	N	N	N	N	R
Site type	HC	PE	HC	HC	PE	GB
Basic monitoring objective(s)	NC, RS, TP	NC, RS, TP	NC, RS, TP	RS	RS	RS, TP
Monitor type	SLAMS	SLAMS	SLAMS	Other	Other	Other
Network affiliation(s), if applicable (a monitor may have none, one, or multiple)	PAMS	PAMS	PAMS, RA40	PAMS	PAMS	PAMS
FRM/FEM/ARM/Other	FEM	FEM	FEM	Other	Other	Other
POC	1	1	1	1	1	1
Primary / QA Collocated / Other (provide for all PM <sub>2.5</sub> , PM <sub>10</sub> , PM <sub>10-2.5</sub> , Pb and NO <sub>2</sub> monitors. Non-PM, Pb, NO <sub>2</sub> monitors should be listed as "N/A".)	N/A	N/A	N/A	N/A	N/A	Other
Is it suitable for comparison against the annual PM <sub>2.5</sub> ? (Y/N)	N/A	N/A	N/A	N/A	N/A	N/A
Instrument manufacturer and model	Teledyne API 400E	Thermo 48i TLE	Teledyne API 200E	Xontech 910/ Xontech 925	Synspec Alpha 115	Many
Analysis method	UV Absorption	Non-dispersive IR	Chem.	GC / UV Absorption	TEI 55: Propane	Many
Method code	087	554	099	177 / 202	011	Many
Monitoring start date (MM/DD/YYYY)	06/01/2012	07/01/2012	07/01/2012	06/01/2012	10/01/2012	07/01/2012
Required sampling frequency (e.g. 1:3 excluding exceptional events/1:1 including exceptional events)	Hourly	Hourly	Hourly	1:3	Hourly	Hourly
Sampling season (MM/DD - MM/DD)	01/01 – 12/31	01/01 – 12/31	01/01 – 12/31	06/01 – 08/31	01/01 – 12/31	01/01 – 12/31
Probe height (meters)	6.0 m	6.0 m	6.0 m	6.3 m	6.0 m	10 m
Distance from supporting structure (meters)	2.1 m	2.1 m	2.1 m	2.4 m	2.1 m	N/A

Pollutant	Ozone	CO	NO <sub>2</sub>	Speciated VOC	NMH	Meteorology
Distance from obstructions on roof. Include horizontal distance + vertical height above probe for obstructions nearby. (meters)	N/A	N/A	N/A	N/A	N/A	N/A
Distance from obstructions not on roof. Include horizontal distance + vertical height above probe for obstructions nearby. (meters)	N/A	N/A	N/A	N/A	N/A	N/A
Distance from trees (meters)	Over 75 m	Over 75 m	Over 75 m	Over 75 m	Over 75 m	Over 75 m
Distance to furnace or incinerator flue (meters)	N/A	N/A	N/A	N/A	N/A	N/A
Distance between monitors fulfilling a QA collocation requirement (meters).	N/A	N/A	N/A	N/A	N/A	N/A
Unrestricted airflow (degrees around probe/inlet or percentage of monitoring path)	350	350	350	350	350	350
Probe material for reactive gases NO/NO <sub>2</sub> /NO <sub>y</sub> , SO <sub>2</sub> , O <sub>3</sub> ; PAMS: VOCs, Carbonyls (e.g. Pyrex, stainless steel, Teflon)	Teflon/Pyrex with Borosilicate	Teflon/Pyrex with Borosilicate	Teflon/Pyrex with Borosilicate	Stainless Steel	Teflon/Pyrex with Borosilicate	N/A
Residence time for reactive gases NO/NO <sub>2</sub> /NO <sub>y</sub> , SO <sub>2</sub> , O <sub>3</sub> ; PAMS: VOCs, Carbonyls (seconds)	11.2	12.3	11.8	4	17.7	N/A
Frequency of one-point QC check for gaseous instruments	Daily	Daily	Daily	N/A	Daily	N/A
Frequency of flow rate verification for manual PM samplers, including Pb samplers (routine checks)	N/A	N/A	N/A	N/A	N/A	N/A
Frequency of flow rate verification for automated PM analyzers (routine checks)	N/A	N/A	N/A	N/A	N/A	N/A
For low volume PM instruments (flow rate < 200 liters/minute), is any PM instrument within 1 m of the level? If yes, please list distance (meters) and instrument(s).	N/A	N/A	N/A	N/A	N/A	N/A

Pollutant	Ozone	CO	NO <sub>2</sub>	Speciated VOC	NMH	Meteorology
For high volume PM instrument (flow rate > 200 liters/minute), is any PM instrument within 2m of the hivol? If yes, please list distance (meters) and instrument(s).	N/A	N/A	N/A	N/A	N/A	N/A
Date of Annual Performance Evaluation conducted in the past calendar year for gaseous parameters (MM/DD/YYYY)	03/22/17	03/22/17	03/22/17	N/A	N/A	N/A
Date of two semi-annual flow rate audits conducted in the past calendar year for PM monitors (MM/DD/YYYY, MM/DD/YYYY)	N/A	N/A	N/A	N/A	N/A	N/A
Changes planned within the next 18 months (Y/N)	N	N	N	N	N	N

<b>Site Name</b>	<b>Bakersfield–Airport (Planz)</b>
<b>AQS ID (XX-XXX-XXXX)</b>	06-029-0016
<b>Representative statistical area Name (i.e. MSA, CBSA, other)</b>	Bakersfield
<b>County</b>	Kern
<b>Collecting (Operating) Agency</b>	CARB
<b>Analytical Lab (i.e. weigh lab, toxics lab, other)</b>	CARB
<b>Reporting Agency</b>	CARB
<b>Site Start Date</b>	09/19/2000
<b>Pollutant Parameters</b>	PM2.5 FRM
<b>Meteorological Parameters</b>	None
<b>Address</b>	401 E. Planz Rd., Bakersfield CA 93307
<b>GPS Coordinates (decimal degrees)</b>	35.3246 N, -118.9976 W
<b>Distance to road</b>	500 m (west)
<b>Traffic Count/Year</b>	17,228/2017 (Traffic count for nearest cross street): S. Union Ave between E. Planz Rd and E White Lane) Source: Kern Council of Governments 1,056/2018 (Traffic count for monitoring station's street address) Source: Kern Council of Governments.
<b>Ground Cover</b>	Paved

<b>Bakersfield–Airport (Planz) (1)</b>	
<b>Pollutant</b>	<b>PM2.5</b>
Parameter code	88101
Spatial scale	N
Site type	PE, HC
Basic monitoring objective(s)	NC, RS
Monitor type	SLAMS
Network affiliation(s), if applicable (a monitor may have none, one, or multiple)	None
FRM/FEM/ARM/Other	FRM
POC	1
Primary / QA Collocated / Other (provide for all PM <sub>2.5</sub> , PM <sub>10</sub> , PM <sub>10-2.5</sub> , Pb and NO <sub>2</sub> monitors. Non-PM, Pb, NO <sub>2</sub> monitors should be listed as "N/A".)	Primary
Is it suitable for comparison against the annual PM <sub>2.5</sub> ? (Y/N)	Y
Instrument manufacturer and model	R&P 2025
Analysis method	Gravimetric
Method code	145
Monitoring start date (MM/DD/YYYY)	09/19/2000
Required sampling frequency (e.g. 1:3 excluding exceptional events/1:1 including exceptional events)	1:3
Sampling season	01/01 – 12/31
Probe Inlet height above ground (meters)	2.0 m
Distance from supporting structure (meters)	None
Distance from obstructions on roof. Include horizontal distance + vertical height above probe for obstructions nearby. (meters)	None
Distance from obstructions not on roof. Include horizontal distance + vertical height above probe for obstructions nearby. (meters)	None
Distance from trees (meters)	None
Distance to furnace or incinerator flue (meters)	None
Distance between collocated monitors (meters)	None
Unrestricted airflow (degrees)	360
Probe material (Teflon, etc.)	N/A
Residence time (seconds)	N/A
For low volume PM instruments (flow rate < 200 liters/minute), is any PM instrument within 1 m of the lovol? If yes, please list distance (meters) and instrument(s).	N/A

<b>Pollutant</b>	<b>PM2.5</b>
For high volume PM instrument (flow rate > 200 liters/minute), is any PM instrument within 2m of the hivol? If yes, please list distance (meters) and instrument(s).	N/A
Frequency of flow rate verification for manual PM samplers audit	Monthly
Frequency of flow rate verification for automated PM analyzers audit	N/A
Frequency of one-point QC check (gaseous)	N/A
Last Annual Performance Evaluation (gaseous)	03/21/2017, 09/20/2017
Last two semi-annual flow rate audits for PM monitors	03/03/2017, 10/05/2017
Changes planned within the next 18 months (Y/N)	Y- Installation of power sub-meter meter and outlet at site.



<b>Site Name</b>	<b>Edison</b>
<b>AQS ID (XX-XXX-XXXX)</b>	06-029-0007
<b>Representative statistical area Name (i.e. MSA, CBSA, other)</b>	Bakersfield
<b>County</b>	Kern
<b>Collecting (Operating) Agency</b>	CARB
<b>Analytical Lab (i.e. weigh lab, toxics lab, other)</b>	N/A
<b>Reporting Agency</b>	CARB
<b>Site Start Date</b>	01/01/1980
<b>Pollutant Parameters</b>	Ozone, NO <sub>2</sub>
<b>Meteorological Parameters</b>	Wind speed, wind direction, outside temperature, relative humidity
<b>Address</b>	Johnston Farms-Shed Rd., Edison, CA 93320
<b>GPS Coordinates (decimal degrees)</b>	35.34561 N, -118.85183 W
<b>Distance to road</b>	450 m (south)
<b>Traffic Count/Year</b>	2,792/2018 (Traffic count for nearest roads: Edison Hwy. and Comanche Dr., Source: Kern Council of Governments.)
<b>Ground Cover</b>	Dirt, vegetative

Edison (1)			
Pollutant	Ozone	NO <sub>2</sub>	Meteorology
Parameter code	44201	42602	61103, 61104, 62102, 62201, 62101
Spatial scale	N	N	R
Site type	HC, RT	PE	GB
Monitoring objective	NC, RS, TP	NC, RS, TP	RS, TP
Monitor type	SLAMS	SLAMS	Other
Network affiliation	SLAMS	SLAMS	SLAMS
FRM/FEM/ARM/Other	FEM	FRM	Other
POC	1	1	1
Primary / QA Collocated / Other (provide for all PM <sub>2.5</sub> , PM <sub>10</sub> , PM <sub>10-2.5</sub> , Pb and NO <sub>2</sub> monitors. Non-PM, Pb, NO <sub>2</sub> monitors should be listed as "N/A".)	N/A	N/A	Primary
Is it suitable for comparison against the annual PM <sub>2.5</sub> ? (Y/N)	N/A	N/A	N/A
Instrument manufacturer and model	Teledyne API 400	Teledyne API 200E	RM Young 81000, Vaisala HMP 155
Analysis method	UV	CL	Sonic, Instrumental
Method code	087	099	066, 059
Monitoring start date (MM/DD/YYYY)	01/01/1981	01/01/1980	01/01/1995
Required sampling frequency (e.g. 1:3 excluding exceptional events/1:1 including exceptional events)	Hourly	Hourly	Hourly
Sampling season (MM/DD - MM/DD)	01/01 – 12/31	01/01 – 12/31	01/01 – 12/31
Probe/Inlet height above ground (meters)	5.4 m	5.4 m	10 m (OT 2.1 m)
Distance from supporting structure (meters)	1.5 m	1.5 m	None
Distance from obstructions on roof. Include horizontal distance + vertical height above probe for obstructions nearby. (meters)	N/A	N/A	N/A
Distance from obstructions not on roof. Include horizontal distance + vertical height above probe for obstructions nearby. (meters)	N/A	N/A	N/A
Distance from trees (meters)	16.1 m (11.0 m to dripline)	16.1 m (11.0 m to dripline)	18.5
Distance to furnace or incinerator flue (meters)	N/A	N/A	N/A
Distance between collocated monitors (meters)	N/A	N/A	N/A
Unrestricted airflow (degrees)	360	360	360

<b>Pollutant</b>	<b>Ozone</b>	<b>NO<sub>2</sub></b>	<b>Meteorology</b>
Probe material (Teflon, etc.)	Teflon	Teflon	N/A
Residence time (seconds)	11.9	14.6	N/A
For low volume PM instruments (flow rate < 200 liters/minute), is any PM instrument within 1 m of the hivol? If yes, please list distance (meters) and instrument(s).	N/A	N/A	N/A
For high volume PM instrument (flow rate > 200 liters/minute), is any PM instrument within 2m of the hivol? If yes, please list distance (meters) and instrument(s).	N/A	N/A	N/A
Frequency of flow rate verification for manual PM samplers audit	N/A	N/A	N/A
Frequency of flow rate verification for automated PM analyzers audit	N/A	N/A	N/A
Frequency of one-point QC check (gaseous)	Daily	Daily	N/A
Last Annual Performance Evaluation (gaseous)	11/02/17	11/02/17	N/A
Last two semi-annual flow rate audits for PM monitors	N/A	N/A	N/A
Changes planned within the next 18 months (Y/N)	N	N	N

<b>Site Name</b>	<b>Arvin–Di Giorgio</b>
<b>AQS ID (XX-XXX-XXXX)</b>	06-029-5002
<b>Representative statistical area Name (i.e. MSA, CBSA, other)</b>	Bakersfield
<b>County</b>	Kern
<b>Collecting (Operating) Agency</b>	CARB
<b>Analytical Lab (i.e. weigh lab, toxics lab, other)</b>	N/A
<b>Reporting Agency</b>	CARB
<b>Site Start Date</b>	11/16/2009
<b>Pollutant Parameters</b>	Ozone
<b>Meteorological Parameters</b>	Outdoor temperature, wind speed, wind direction, sonic temperature, relative humidity
<b>Address</b>	19405 Buena Vista Blvd, Arvin CA 93203
<b>GPS Coordinates (decimal degrees)</b>	35.2391 N, -118.7886 W
<b>Distance to road</b>	10 m (east)
<b>Traffic Count/Year</b>	598/2016 (Traffic count for Buena Vista Blvd east of Tejon Hwy., Source: Kern Council of Governments.)
<b>Ground Cover</b>	Dirt, vegetative

<b>Arvin-Di Giorgio (1)</b>		
<b>Pollutant</b>	<b>Ozone</b>	<b>Meteorology</b>
Parameter code	44201	61104, 61103, 62101, 62102, 62201
Spatial scale	N	R
Site type	HC, PE	GB
Monitor objective	NC, RS, TP	RS, TP
Monitor type	SLAMS	SLAMS (WD, WS), Other (OT, RH)
Network affiliation	PAMS (pending)	PAMS (pending)
FRM/FEM/ARM/Other	FEM	Other
POC	1	2
Primary / QA Collocated / Other (provide for all PM <sub>2.5</sub> , PM <sub>10</sub> , PM <sub>10-2.5</sub> , Pb and NO <sub>2</sub> monitors. Non-PM, Pb, NO <sub>2</sub> monitors should be listed as "N/A".)	N/A	Other
Is it suitable for comparison against the annual PM <sub>2.5</sub> ? (Y/N)	N/A	N/A
Instrument manufacturer and model	Teledyne API 400E	RM Young 81000, Vaisala HMP155
Analysis method	UV	Sonic
Method code	087	066, 059
Monitoring start date (MM/DD/YYYY)	11/16/2009	11/16/2009, 9/2/2015 (Vaisala)
Required sampling frequency (e.g. 1:3 excluding exceptional events/1:1 including exceptional events)	Hourly	Hourly
Sampling season (MM/DD - MM/DD)	01/01 – 12/31	01/01 – 12/31
Probe height (meters)	4.4 m	10 m
Distance from supporting structure (meters)	1.8 m	N/A
Distance from obstructions on roof. Include horizontal distance + vertical height above probe for obstructions nearby. (meters)	N/A	N/A
Distance from obstructions not on roof. Include horizontal distance + vertical height above probe for obstructions nearby. (meters)	N/A	N/A
Distance from trees (meters)	>10 m	18.5 m
Distance to furnace or incinerator flue (meters)	N/A	N/A
Distance between collocated monitors (meters)	N/A	N/A
Unrestricted airflow (degrees)	360	360
Probe material (Teflon, etc.)	TEFLON	Teflon
Residence time (seconds)	14.56	N/A
For low volume PM instruments (flow rate < 200 liters/minute), is any PM instrument within 1 m of the loval? If yes, please list distance (meters) and instrument(s).	N/A	N/A

<b>Pollutant</b>	<b>Ozone</b>	<b>Meteorology</b>
For high volume PM instrument (flow rate > 200 liters/minute), is any PM instrument within 2m of the hivol? If yes, please list distance (meters) and instrument(s).	N/A	N/A
Frequency of flow rate verification for manual PM samplers audit	N/A	N/A
Frequency of flow rate verification for automated PM analyzers audit	N/A	N/A
Frequency of one-point QC check (gaseous)	Daily	N/A
Last Annual Performance Evaluation (gaseous)	12/13/2017	N/A
Last two semi-annual flow rate audits for PM monitors	N/A	N/A
Changes planned within the next 18 months (Y/N)	N	N

<b>Site Name</b>	<b>Maricopa</b>
<b>AQS ID (XX-XXX-XXXX)</b>	06-029-0008
<b>Representative statistical area Name (i.e. MSA, CBSA, other)</b>	Bakersfield
<b>County</b>	Kern
<b>Collecting (Operating) Agency</b>	SJVAPCD
<b>Analytical Lab (i.e. weigh lab, toxics lab, other)</b>	N/A
<b>Reporting Agency</b>	SJVAPCD
<b>Site Start Date</b>	7/1/1987
<b>Pollutant Parameters</b>	Ozone
<b>Meteorological Parameters</b>	Wind speed, wind direction, outdoor temperature, barometric pressure
<b>Address</b>	755 Stanislaus St., Maricopa, CA 93252
<b>GPS Coordinates (decimal degrees)</b>	35.0515 N, -119.4026 W
<b>Distance to roadways (meters)</b>	500 (northwest)
<b>Traffic Count/Year</b>	267/2017 (Traffic count for nearest roads: Union St. at California St., Source: Kern Council of Governments.)
<b>Groundcover (e.g. paved, vegetative, dirt, sand, gravel)</b>	Gravel, dirt, vegetative

<b>Maricopa (1)</b>		
<b>Pollutant</b>	<b>Ozone</b>	<b>Meteorology</b>
Parameter code	44201	Many
Spatial scale	N	N
Site type	HC, RT	GB
Basic monitoring objective(s)	NC, RS, TP	RS, TP
Monitor type	SLAMS	Other
Network affiliation(s), if applicable (a monitor may have none, one, or multiple)	None	None
FRM/FEM/ARM/Other	FEM	Other
POC	1	1
Primary / QA Collocated / Other (provide for all PM <sub>2.5</sub> , PM <sub>10</sub> , PM <sub>10-2.5</sub> , Pb and NO <sub>2</sub> monitors. Non-PM, Pb, NO <sub>2</sub> monitors should be listed as "N/A".)	N/A	Other
Is it suitable for comparison against the annual PM <sub>2.5</sub> ? (Y/N)	N/A	N/A
Instrument manufacturer and model	Teledyne API 400E	ITP- Hy-Cal 512AA3B, OT- Met One 060A-2, BP- Met One 092, WD- Met One 020C, WS-Met One 010C
Analysis method	UV	Many
Method code	087	Many
Monitoring start date (MM/DD/YYYY)	07/01/1987	07/01/1987
Required sampling frequency (e.g. 1:3 excluding exceptional events/1:1 including exceptional events)	Hourly	Hourly
Sampling season (MM/DD - MM/DD)	01/01 – 12/31	01/01 – 12/31
Probe height (meters)	3.0 m	10 m
Distance from supporting structure (meters)	1.0 m	N/A
Distance from obstructions on roof. Include horizontal distance + vertical height above probe for obstructions nearby. (meters)	3 m H 0.5 m V	N/A
Distance from obstructions not on roof. Include horizontal distance + vertical height above probe for obstructions nearby. (meters)	17 m H 1 m V	N/A
Distance from trees (meters)	18 m H 8 m V	20 m
Distance to furnace or incinerator flue (meters)	N/A	N/A
Distance between monitors fulfilling a QA collocation requirement (meters).	N/A	N/A
Unrestricted airflow (degrees around probe/inlet or percentage of monitoring path)	350	360



Pollutant	Ozone	Meteorology
Probe material for reactive gases NO/NO <sub>2</sub> /NO <sub>y</sub> , SO <sub>2</sub> , O <sub>3</sub> ; PAMS: VOCs, Carbonyls (e.g. Pyrex, stainless steel, Teflon)	Teflon/Pyrex with Borosilicate	N/A
Residence time for reactive gases NO/NO <sub>2</sub> /NO <sub>y</sub> , SO <sub>2</sub> , O <sub>3</sub> ; PAMS: VOCs, Carbonyls (seconds)	7.34	N/A
Frequency of one-point QC check for gaseous instruments	Daily	N/A
Frequency of flow rate verification for manual PM samplers, including Pb samplers (routine checks)	N/A	N/A
Frequency of flow rate verification for automated PM analyzers (routine checks)	N/A	N/A
For low volume PM instruments (flow rate < 200 liters/minute), is any PM instrument within 1 m of the hivol? If yes, please list distance (meters) and instrument(s).	N/A	N/A
For high volume PM instrument (flow rate > 200 liters/minute), is any PM instrument within 2m of the hivol? If yes, please list distance (meters) and instrument(s).	N/A	N/A
Date of Annual Performance Evaluation conducted in the past calendar year for gaseous parameters (MM/DD/YYYY)	10/31/17	N/A
Date of two semi-annual flow rate audits conducted in the past calendar year for PM monitors (MM/DD/YYYY, MM/DD/YYYY)	N/A	N/A
Changes planned within the next 18 months (Y/N)	N	N

<b>Site Name</b>	<b>Lebec</b>
<b>AQS ID (XX-XXX-XXXX)</b>	06-029-2009
<b>Representative statistical area Name (i.e. MSA, CBSA, other)</b>	Bakersfield
<b>County</b>	Kern
<b>Collecting (Operating) Agency</b>	SJVAPCD
<b>Analytical Lab (i.e. weigh lab, toxics lab, other)</b>	N/A
<b>Reporting Agency</b>	SJVAPCD
<b>Site Start Date</b>	1/20/2009
<b>Pollutant Parameters</b>	PM2.5 Non-FEM
<b>Meteorological Parameters</b>	Wind speed, wind direction, outdoor temperature, barometric pressure
<b>Address</b>	1277 Beartrap Road, Lebec, CA 93243
<b>GPS Coordinates (decimal degrees)</b>	34.8415N, -118.8610W
<b>Distance to roadways (meters)</b>	300 m (west)
<b>Traffic Count/Year</b>	1,911/2017 (Traffic count for nearest roads: Lebec Rd near Interstate 5, Source: Kern Council of Governments.)
<b>Groundcover (e.g. paved, vegetative, dirt, sand, gravel)</b>	Gravel, vegetative

<b>Lebec</b>		
<b>Pollutant</b>	<b>PM2.5</b>	<b>Meteorology</b>
Parameter code	88502	Many
Spatial scale	N	R
Site type	PE	GB
Basic monitoring objective(s)	TP	RS, TP
Monitor type	SPM	Other
Network affiliation(s), if applicable (a monitor may have none, one, or multiple)	None	None
FRM/FEM/ARM/Other	Non-FEM	Other
POC	3	1
Primary / QA Collocated / Other (provide for all PM <sub>2.5</sub> , PM <sub>10</sub> , PM <sub>10-2.5</sub> , Pb and NO <sub>2</sub> monitors. Non-PM, Pb, NO <sub>2</sub> monitors should be listed as "N/A".)	Primary	Other
Is it suitable for comparison against the annual PM <sub>2.5</sub> ? (Y/N)	N	N/A
Instrument manufacturer and model	MET One BAM 1020	ITP- Hy-Cal 512AA3B, OT- Met One 060A-2, BP- Met One 092, WD- Met One 020C, WS-Met One 010C
Analysis method	Beta Attenuation	Many
Method code	731	Many
Monitoring start date (MM/DD/YYYY)	01/27/2009	OT, WS, WD - 12/09/2009; BP – 01/28/2010
Required sampling frequency (e.g. 1:3 excluding exceptional events/1:1 including exceptional events)	Hourly	Hourly
Sampling season (MM/DD - MM/DD)	01/01 -12/31	01/01 – 12/31
Probe height (meters)	1.98 m	10 m
Distance from supporting structure (meters)	4.62 m	N/A
Distance from obstructions on roof. Include horizontal distance + vertical height above probe for obstructions nearby. (meters)	N/A	N/A
Distance from obstructions not on roof. Include horizontal distance + vertical height above probe for obstructions nearby. (meters)	N/A	N/A
Distance from trees (meters)	200 m	200 m
Distance to furnace or incinerator flue (meters)	N/A	N/A
Distance between monitors fulfilling a QA collocation requirement (meters).	N/A	N/A
Unrestricted airflow (degrees around probe/inlet or percentage of monitoring path)	360	360

<b>Pollutant</b>	<b>PM2.5</b>	<b>Meteorology</b>
Probe material for reactive gases NO/NO <sub>2</sub> /NO <sub>y</sub> , SO <sub>2</sub> , O <sub>3</sub> ; PAMS: VOCs, Carbonyls (e.g. Pyrex, stainless steel, Teflon)	N/A	N/A
Residence time for reactive gases NO/NO <sub>2</sub> /NO <sub>y</sub> , SO <sub>2</sub> , O <sub>3</sub> ; PAMS: VOCs, Carbonyls (seconds)	N/A	N/A
Frequency of one-point QC check for gaseous instruments	N/A	N/A
Frequency of flow rate verification for manual PM samplers, including Pb samplers (routine checks)	N/A	N/A
Frequency of flow rate verification for automated PM analyzers (routine checks)	Monthly	N/A
For low volume PM instruments (flow rate < 200 liters/minute), is any PM instrument within 1 m of the lovol? If yes, please list distance (meters) and instrument(s).	No	N/A
For high volume PM instrument (flow rate > 200 liters/minute), is any PM instrument within 2m of the hivol? If yes, please list distance (meters) and instrument(s).	N/A	N/A
Date of Annual Performance Evaluation conducted in the past calendar year for gaseous parameters (MM/DD/YYYY)	N/A	N/A
Date of two semi-annual flow rate audits conducted in the past calendar year for PM monitors (MM/DD/YYYY, MM/DD/YYYY)	04/05/17, 10/23/17	N/A
Changes planned within the next 18 months (Y/N)	N	N

**APPENDIX C:**

**San Joaquin Valley Air Pollution Control District Notice of Public  
Inspection Period on the 2018 Air Monitoring Network Plan**

This page intentionally blank

**SAN JOAQUIN VALLEY UNIFIED AIR POLLUTION CONTROL DISTRICT  
NOTICE OF PUBLIC INSPECTION PERIOD ON THE  
DRAFT 2018 AIR MONITORING NETWORK PLAN**

NOTICE IS HEREBY GIVEN that a 30-day public inspection period is being held on the San Joaquin Valley Air Pollution Control District's (District) Draft 2018 Air Monitoring Network Plan.

Interested persons may submit comments to:

Robert Gilles  
San Joaquin Valley Unified Air Pollution Control District  
1990 East Gettysburg Avenue  
Fresno, CA 93726  
Email: [robert.gilles@valleyair.org](mailto:robert.gilles@valleyair.org)

The public inspection period begins May 29, 2018 and will end June 28, 2018.

Copies of the Draft 2018 Air Monitoring Network Plan can be obtained by calling (559) 230-6100. You may download a copy of the Draft 2018 Air Monitoring Network Plan from the District's website on or after May 29, 2018 under the Other Notices portion of the Public Notices page:

[http://www.valleyair.org/notices/public\\_notices\\_idx.htm#Other Notices](http://www.valleyair.org/notices/public_notices_idx.htm#Other Notices)

For additional information, contact Robert Gilles by phone at (559) 230-6100.